



## LABORATORY FOR PRODUCTION MEASUREMENT

Faculty of Mechanical Engineering  
Smetanova 17, 2000 Maribor, Slovenia

# QUALITY MANUAL

Issue date	27. 2. 2024
Issue No.	E-30
Authors	Prof. Dr. Bojan Ačko Dr. Jasna Tompa
Approved by	Prof. Dr. Bojan Ačko

**Evidence of changes (regarding the previous issue)**

Amendment No.	Changed Chapter	Removed Chapter	Added Chapter
1	<a href="#">1.3.4</a>		
2	<a href="#">2.4</a>		
3	<a href="#">3.3</a>		
4	<a href="#">5.1</a>		
5	<a href="#">6.1</a>		
6	<a href="#">9.1.1</a>		
7	<a href="#">10</a>		
8	<a href="#">12.1</a>		
9	<a href="#">13.2.3</a>		
10	<a href="#">18</a>		

# Contents

<b>1</b>	<b>INTRODUCTION OF THE LABORATORY</b>	<b>7</b>
<b>1.1</b>	<b>General information about the laboratory</b>	<b>7</b>
1.1.1	The limits in which the laboratory is working:	7
<b>1.2</b>	<b>Functions and technical scope</b>	<b>8</b>
1.2.1	Fields of work	8
1.2.2	Technological sectors to which our activities apply	8
1.2.3	Clients	8
1.2.4	Geographical areas where the activities take place	8
1.2.5	Technical scope of the laboratory	8
1.2.6	National standard	9
<b>1.3</b>	<b>Relationship to parent organization</b>	<b>9</b>
1.3.1	Main activities of the University of Maribor (parent organization)	9
1.3.2	Organizational Chart of the University of Maribor	9
1.3.3	Organizational Chart of the Faculty of Mechanical Engineering	9
1.3.4	Organizational Chart of the Mechanical Engineering Research Institute	10
1.3.5	Influence of the University and the Faculty of mechanical engineering on the functioning of the laboratory	11
<b>2</b>	<b>QUALITY POLICY</b>	<b>12</b>
<b>2.1</b>	<b>Quality policy, the objectives, the management's involvement with quality</b>	<b>12</b>
<b>2.2</b>	<b>Assurance of independence, impartiality and integrity</b>	<b>13</b>
2.2.1	Risk and opportunities identified	13
<b>2.3</b>	<b>Policy regarding protection of staff against improper influencing</b>	<b>13</b>
<b>2.4</b>	<b>Assurance of security of information</b>	<b>13</b>
<b>3</b>	<b>ORGANIZATION AND MANAGEMENT</b>	<b>14</b>
<b>3.1</b>	<b>Organizational structure of the Laboratory for production measurement</b>	<b>14</b>
<b>3.2</b>	<b>Description of activities in the departments</b>	<b>15</b>
3.2.1	Department »Measurements and calibration«	15
3.2.2	Department »Development of new measuring devices«	15
3.2.3	Department »Education, training of experts«	15
3.2.4	Department »Research (dimensional metrology, quality assurance) «	16
<b>3.3</b>	<b>Managers and their deputies</b>	<b>17</b>
<b>3.4</b>	<b>Management in the absence of manager(s)</b>	<b>17</b>
<b>3.5</b>	<b>Supervision of personnel</b>	<b>17</b>
3.5.1	Procedure for supervising the permanent personnel	17
3.5.2	Procedure for supervising the personnel which is not yet (fully) qualified	18
<b>3.6</b>	<b>Job description</b>	<b>18</b>
3.6.1	Procedure for preparing job descriptions	18
3.6.2	Procedures for amending job descriptions	19
3.6.3	Procedures for the case, when workers are not performing their work according to requirements	20
<b>4</b>	<b>QUALITY SYSTEM</b>	<b>21</b>
<b>4.1</b>	<b>Responsibilities</b>	<b>21</b>
4.1.1	Responsibility of the laboratory for quality of the work performed	21
4.1.2	Insurance of the laboratory responsibility	21
4.1.3	Personal responsibilities	21
<b>4.2</b>	<b>Quality manager</b>	<b>21</b>
<b>4.3</b>	<b>Arrangements for permitting departures from documented policies and procedures or from standard specifications</b>	<b>21</b>
<b>5</b>	<b>DOCUMENTATION</b>	<b>23</b>
<b>5.1</b>	<b>Location and names of the files</b>	<b>23</b>
<b>5.2</b>	<b>Access to the files</b>	<b>24</b>
<b>5.3</b>	<b>Drafting, changing, approving, validity and archiving of documents</b>	<b>24</b>
<b>5.4</b>	<b>Protection from the use of obsolete/superseded documentation</b>	<b>25</b>

<b>5.5</b>	<b>Rule for identification of issues</b>	<b>25</b>
<b>5.6</b>	<b>Changes in the documents and new issues</b>	<b>25</b>
<b>5.7</b>	<b>Procedures for protecting data from loss</b>	<b>25</b>
<b>5.8</b>	<b>External documents</b>	<b>25</b>
<b>6</b>	<b>REPORTS AND RECORDS</b>	<b>27</b>
<b>6.1</b>	<b>Reports</b>	<b>27</b>
6.1.1	Calibration reports	27
6.1.2	Instructions for amending/supplementing reports	27
6.1.3	Instructions for distributing copies of the records	27
<b>6.2</b>	<b>Records</b>	<b>27</b>
6.2.1	List of records	28
6.2.2	Indexing, storage and archiving records on paper	28
6.2.3	Indexing, storage and archiving of electronic records	29
6.2.4	Procedure for lending out the filed records	29
6.2.5	Guidelines for changing records	29
<b>7</b>	<b>QUALITY SYSTEM CONTROL</b>	<b>30</b>
<b>7.1</b>	<b>Internal quality audits</b>	<b>30</b>
7.1.1	Guidelines for performing internal quality audits	30
7.1.2	Planning of the internal quality audits	30
7.1.3	Instructions/checklists for performing audits	30
7.1.4	Audit report	30
7.1.5	Nonconformance and corrective actions	30
<b>7.2</b>	<b>Management review</b>	<b>30</b>
<b>7.3</b>	<b>Quality system control during the work</b>	<b>31</b>
7.3.1	Procedures for reporting and registering nonconformities	31
7.3.2	Procedures for execution of corrective actions	31
7.3.3	Procedure for analysing deficiencies, complaints etc. and for investigating their causes	32
7.3.4	Procedure for checking whether work is required to be either wholly or partially redone	32
<b>8</b>	<b>PERSONNEL</b>	<b>34</b>
<b>8.1</b>	<b>Policy regarding the personnel performing calibrations</b>	<b>34</b>
<b>8.2</b>	<b>Selection and recruitment</b>	<b>34</b>
8.2.1	Procedure for recruiting and selecting personnel	34
8.2.2	Procedure for hiring temporary personnel	35
<b>8.3</b>	<b>Education</b>	<b>35</b>
8.3.1	Procedure for training new staff	35
8.3.2	Procedure regarding the periodic checks of staff qualification	36
8.3.3	Description of the training system	36
<b>8.4</b>	<b>Documentation</b>	<b>37</b>
8.4.1	Instructions on keeping the personal files	37
<b>9</b>	<b>FACILITIES</b>	<b>38</b>
<b>9.1</b>	<b>Using the special installations</b>	<b>38</b>
9.1.1	Operating instructions for special installations	38
<b>9.2</b>	<b>Access and use of spaces and installations</b>	<b>38</b>
9.2.1	Access to the spaces and installations	38
9.2.2	Instructions for the use of spaces	39
<b>9.3</b>	<b>Climatic conditions in the laboratory</b>	<b>40</b>
9.3.1	Reference conditions	40
9.3.2	Registering conditions	40
<b>10</b>	<b>EQUIPMENT</b>	<b>41</b>
<b>10.1</b>	<b>Policy for achieving traceability of measurements</b>	<b>41</b>
<b>10.2</b>	<b>Identification and evidence</b>	<b>41</b>
10.2.1	Equipment file	41
10.2.2	Identification of measuring equipment	43
10.2.3	Instructions for keeping the equipment files	43

<b>10.3</b>	<b>Issue and receipt</b>	<b>43</b>
10.3.1	Procedures for supervision, issue and receipt of equipment	43
10.3.2	Rules for borrowing equipment from third parties	44
<b>10.4</b>	<b>Authority</b>	<b>44</b>
10.4.1	Rules regarding the authority to use the equipment	44
<b>10.5</b>	<b>Equipment locations</b>	<b>44</b>
<b>10.6</b>	<b>Maintenance</b>	<b>45</b>
10.6.1	Maintenance instructions	45
10.6.2	Lists of spare parts	45
<b>10.7</b>	<b>Calibration</b>	<b>45</b>
10.7.1	Procedures for calibration of the equipment	45
10.7.2	Program for performing periodic calibrations	46
10.7.3	Analysis of calibration results	46
10.7.4	Intermediate checks	47
<b>10.8</b>	<b>Computer system</b>	<b>47</b>
10.8.1	Documentation of the computer system	47
<b>10.9</b>	<b>Defective equipment</b>	<b>48</b>
10.9.1	Instruction for removing defective equipment from use	48
<b>11</b>	<b>SUPPLIES AND SERVICES</b>	<b>49</b>
<b>11.1</b>	<b>Purchasing and contract service policy</b>	<b>49</b>
<b>11.2</b>	<b>Suppliers</b>	<b>49</b>
11.2.1	Procedure for the assessment of suppliers	49
<b>11.3</b>	<b>Documentation</b>	<b>50</b>
11.3.1	Procedure for drafting, checking and approval of purchasing documents	50
<b>11.4</b>	<b>Receipt and inspection</b>	<b>51</b>
11.4.1	Procedure for the receipt and inspection of purchased products	51
11.4.2	Inspection instructions for incoming products	52
<b>11.5</b>	<b>Service check</b>	<b>52</b>
11.5.1	Procedure and instructions for checking services	52
<b>11.6</b>	<b>Storage</b>	<b>53</b>
11.6.1	Procedures for receipt, storage and issue of products, for stock control and for checking products on stock	53
<b>12</b>	<b>PERFORMANCE OF THE WORK</b>	<b>54</b>
<b>12.1</b>	<b>Review of requests, tenders and contracts</b>	<b>54</b>
<b>12.2</b>	<b>Performing the work</b>	<b>55</b>
<b>12.3</b>	<b>Policy regarding design and development activities</b>	<b>56</b>
<b>12.4</b>	<b>Calibration procedures</b>	<b>57</b>
<b>12.5</b>	<b>Validation of the software used for calibration</b>	<b>57</b>
<b>12.6</b>	<b>Quality control of performed work</b>	<b>57</b>
12.6.1	Intercomparisons	57
<b>12.7</b>	<b>Work instructions</b>	<b>58</b>
12.7.1	List of available work instructions	58
12.7.2	Documentation	58
<b>12.8</b>	<b>Security</b>	<b>58</b>
12.8.1	Protection against unauthorized entering the measuring rooms	58
12.8.2	Instructions on how to act in the case of emergency	58
12.8.3	Instructions for the use of personal safety equipment	58
<b>12.9</b>	<b>Objects of calibration</b>	<b>59</b>
12.9.1	Procedures for receipt, storage and issue of calibration objects	59
12.9.2	Identification system for calibration objects	59
12.9.3	Handling of calibration objects	60
12.9.4	Procedures for storing objects of calibration	60
12.9.5	Procedures for delivering objects of calibration	60
<b>12.10</b>	<b>Software for calibration</b>	<b>61</b>

12.10.1	Procedure for maintaining and up-dating software for calibrations	61
12.10.2	Procedure for filing changed (old) versions of calibration software	61
<b>13</b>	<b>CALIBRATION ON SITE</b>	<b>62</b>
<b>13.1</b>	<b>Quality policy</b>	<b>62</b>
<b>13.2</b>	<b>Organization</b>	<b>62</b>
13.2.1	Organization scheme	62
13.2.2	Personnel	62
13.2.3	Equipment	62
13.2.4	Procedures	62
<b>13.3</b>	<b>Planning of calibration</b>	<b>63</b>
<b>13.4</b>	<b>Performance of calibration</b>	<b>63</b>
<b>13.5</b>	<b>Activities after calibration</b>	<b>64</b>
<b>13.6</b>	<b>Audit and review</b>	<b>65</b>
13.6.1	Audit of performance of calibration on site	65
13.6.2	Management review	65
<b>14</b>	<b>SUBCONTRACTING</b>	<b>66</b>
<b>14.1</b>	<b>Policy regarding subcontracting</b>	<b>66</b>
<b>14.2</b>	<b>Procedure for subcontracting calibrations</b>	<b>66</b>
<b>14.3</b>	<b>List of accredited subcontractors</b>	<b>66</b>
<b>14.4</b>	<b>List of subcontracted calibrations</b>	<b>66</b>
<b>15</b>	<b>COOPERATION WITH CLIENTS</b>	<b>67</b>
<b>15.1</b>	<b>Visits in the laboratory and communication with clients</b>	<b>67</b>
<b>15.2</b>	<b>Evaluation of client's satisfaction</b>	<b>67</b>
<b>16</b>	<b>COMPLAINTS</b>	<b>68</b>
<b>16.1</b>	<b>Procedure for dealing with complaints</b>	<b>68</b>
<b>16.2</b>	<b>Instructions for keeping the register of complaints</b>	<b>69</b>
<b>17</b>	<b>COOPERATION WITH ACCREDITATION BODIES, CALIBRATION INSTITUTIONS AND AUTHORITIES</b>	<b>70</b>
<b>18</b>	<b>SCOPE OF ACCREDITATION ACCORDING TO ISO 17025:2017</b>	<b>71</b>

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>7 of 79</b>
	<b>Introduction of the laboratory</b>	Issue No. <b>E-30</b>

# 1 INTRODUCTION OF THE LABORATORY

## 1.1 General information about the laboratory

Statutory name:	Laboratorij za tehnološke meritve (Laboratory for Production Measurement)	
Abbreviation:	LTM	
Legal status:	The laboratory is not a legal body (a legal body is University of Maribor). It is a part of the Mechanical Engineering Research Institute (the Institute is a body inside the Faculty of Mechanical Engineering with unlimited authority regarding all work except education).	
Register No.:	University of Maribor (parent organization):	5229901000
	Faculty of Mechanical Engineering:	5085462 005
	Laboratory of production measurement:	0795-002
Address:	Laboratory for Production Measurement Faculty of Mechanical Engineering Smetanova 17, 2000 Maribor Slovenia	
Telephone No.:	(+386) 2 220 7581, prof. dr. Bojan Ačko, Head of the LTM	
	02 220 7608, Dr. Rok Klobučar, assistant	
	02 220 7762, Dr. Lucija Črepinšek Lipuš, assistant	
	02 220 7913, Dr. Jasna Tompa, assistant	
	02 220 7587, calibration laboratory	
	02 220 7522, secretary's office	
Fax No.:	02220-7990	
Internet:	<a href="https://ltm.fs.um.si/">https://ltm.fs.um.si/</a>	
E-mail:	<a href="mailto:ltm@um.si">ltm@um.si</a> <a href="mailto:bojan.acko@um.si">bojan.acko@um.si</a> <a href="mailto:mitja.mlakar@um.si">mitja.mlakar@um.si</a> <a href="mailto:lucija.crepinsek-lipus@um.si">lucija.crepinsek-lipus@um.si</a> <a href="mailto:rok.klobucar@um.si">rok.klobucar@um.si</a> <a href="mailto:jasna.tompa@um.si">jasna.tompa@um.si</a>	
Operating conditions:	Published on the LTM web page (information for clients under section »Calibration and measurement«)	

### 1.1.1 The limits in which the laboratory is working:

- the best measuring capability expressed as uncertainty: Q[35, 0.5L], L in mm
- the greatest measuring range: (800 x 1000 x 500) mm (3D)  
30 m (1D - laser interferometer).

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>8</b> of <b>79</b>
	<b>Introduction of the laboratory</b>	Issue No. <b>E-30</b>

## **1.2 Functions and technical scope**

### **1.2.1 Fields of work**

Work in the laboratory is divided in the following fields:

- calibration of measuring devices for lengths and angles,
- realization, storing and maintenance of the national standard for length,
- inspection and measurement for industry (especially coordinate measuring technique),
- education (undergraduate and graduate study),
- training of experts,
- research and development of new measuring methods and devices,
- research in the field of dimensional measuring technique and CAQ.

### **1.2.2 Technological sectors to which our activities apply**

Our activities apply to the sectors of quality assurance, production measurement and manufacturing.

### **1.2.3 Clients**

Our clients are industrial and trading companies, companies offering services, institutes, laboratories, universities and ministries.

### **1.2.4 Geographical areas where the activities take place**

The activities take place in the Republic of Slovenia and in smaller amount on European market.

### **1.2.5 Technical scope of the laboratory**

The following methods and procedures are used at our work:

- standard methods of coordinate measuring technique (CMMA, DIN, ISO, ANSI),
- standard and own methods of conventional measuring technique (1D, 2D),
- standard methods of laser interferometry (inspection of machine tools and measuring machines),
- standardized procedures of calibration of measuring devices and standards of measurement (ISO, DIN, ANSI, ...),
- standardized methods for expressing measuring uncertainty (WECC, ISO, DIN, EA, ...),
- finite element method,
- analytical geometry,
- design and technology for production of measuring devices,
- statistical evaluation of measuring results, ...

The limits in which the laboratory is working are stated in chapter 1.1.1.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>9</b> of <b>79</b>
	<b>Introduction of the laboratory</b>	Issue No. <b>E-30</b>

### 1.2.6 National standard

The laboratory (res. legal entity is University of Maribor – Faculty of Mechanical Engineering) is keeping and maintaining the national standard of length. The relation to the National Metrology Institute is regulated with the »Provision about the recognition of the standard as national standard«, issued by the Slovenian Metrology Institute (MIRS) under number 535-1/98-26, and with the yearly Annex to the contract between MIRS and LTM. The laboratory is responsible for realization, storing and maintaining the national standard and for assuring its traceability to international level (to BIPM standards). Performance of the work in the field of the national standard is based on identified current and future national needs and on the requirements of the Slovenian Metrology Institute, defined in the two documents stated above.

Laboratory enables Slovenian industry to perform internationally comparable measurements in the field »length« and herewith better competitive position.

## 1.3 Relationship to parent organization

### 1.3.1 Main activities of the University of Maribor (parent organization)

- education,
- scientific research,
- technological help to industry, tourism and agriculture,
- development of new technologies,
- development of new products,
- metrology.

### 1.3.2 Organizational Chart of the University of Maribor

Organizational Chart of the University of Maribor is available at

<http://pisjboss.um.si:8080/hrm/planizo/objavljenaSistemizacijaDm.xhtml>

### 1.3.3 Organizational Chart of the Faculty of Mechanical Engineering

Organizational Chart of the Faculty of Mechanical Engineering is available at


<http://www.fs.um.si/o-nas/organiziranost/>

	<b>QUALITY MANUAL</b>	Page No.: <b>10</b> of <b>79</b>
	<b>Introduction of the laboratory</b>	Issue No. <b>E-30</b>

### 1.3.4 Organizational Chart of the Mechanical Engineering Research Institute

Laboratories of the Mechanical Engineering Research Institute are available at

<https://www.fs.um.si/en/about-us/faculty-organisation/chairs-institute-centers/mechanical-engineering-research-institute/>

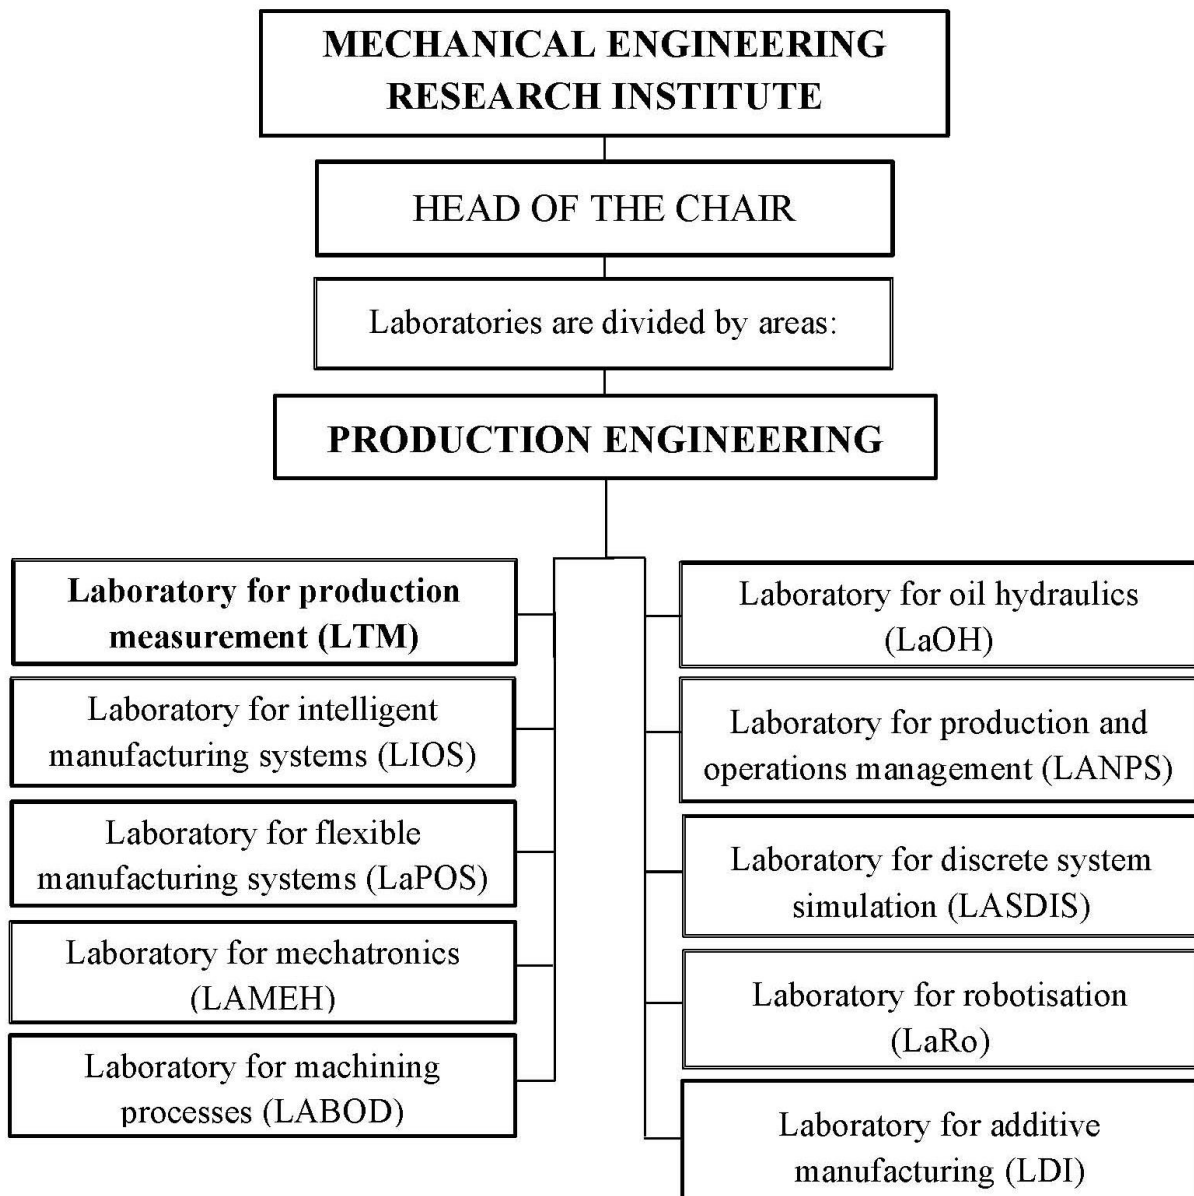

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>11</b> of <b>79</b>
	<b>Introduction of the laboratory</b>	Issue No. <b>E-30</b>

### **1.3.5 Influence of the University and the Faculty of mechanical engineering on the functioning of the laboratory**

The university has no influence on the quality system, finances and the personnel policy of the laboratory. All authorities regarding the functioning of the laboratory has the Faculty of mechanical engineering. The faculty controls the following activities of the laboratory:

- program of education,
- financial state,
- salaries (basic regulations),
- employment (basic conditions and regulation for employment).

All other functioning aspects are under the authority of the laboratory. The financial decisions (purchase of equipment, service charges, stimulation of the staff) are also taken on the laboratory level. The faculty can limit financial actions only in the case of negative financial state of the laboratory.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>12</b> of <b>79</b>
	<b>Quality policy</b>	Issue No. <b>E-30</b>

## 2 QUALITY POLICY

### 2.1 Quality policy, the objectives, the management's involvement with quality

Our quality policy is based on the following objectives:

- satisfaction of client's requirements,
- proper uncertainty of measurement and calibration,
- performance of measurements, calibrations on time,
- confidentiality of data and impartiality, independence and integrity in all fields of work,
- competitive prices,
- safety during performance of the work (staff, equipment, objects of calibration and measurement, documentation).

Beside these objectives, the quality system should also assure:

- well feeling of the staff,
- staff affiliation to the laboratory,
- longer life of the equipment,
- maintenance of the laboratory quality level.

In order to fulfil the quality objectives, we have introduced a quality assurance system, which is precisely defined by the quality manual and the supporting documentation. The quality system is designed in such way, that all requirements of the standard ISO/IEC 17025:2017 are met. It is based on the properly qualified and informed staff, precisely defined extent of work, proper equipment (right selection, maintenance, and traceability) and facilities (according to the requirements of ISO standard), and precisely defined work procedures and instructions. The quality policy require continuous learning of the staff, continuous control (audits, checks, ...) and reviews of the quality system, total control of documentation and records, continuous detection and correction of deficiencies, selection of the most suitable and economic work methods, and regular maintenance of the equipment and the facilities. The laboratory management is fully responsible for the quality of work in the laboratory on all levels and for the conformance of the quality system with the standard ISO/IEC 17025:2017. The laboratory manager is personally responsible for fulfilling the requirements of the quality policy. The quality manager is personally responsible for the control (audits, checks ...) and the review of the quality system. The laboratory staff performing calibration shall always be familiar with the valid versions of the quality system documentation and shall act in conformance with defined policy and procedures. The laboratory and its staff shall consider principles of independence, impartiality and integrity regarding the policy in chapter 2.2.

Quality policy was defined by the laboratory manager and approved by the dean of the Faculty of Mechanical Engineering. Signed original is in »Z 09 - Izjave in pooblastila«.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>13</b> of <b>79</b>
	<b>Quality policy</b>	Issue No. <b>E-30</b>

## 2.2 Assurance of independence, impartiality and integrity

All laboratory employees are shell, while performing their work, respect the principles of independence, impartiality and integrity. They are obliged to act so by a signed statement. The statements are kept in »P 01 – Personnel files«. If it is found out that a person does not respect the above principles, a disciplinary procedure, respecting legal acts of the Faculty, is initiated.

### 2.2.1 Risk and opportunities identified

The risks for the execution of the calibration activity always need to be identified. Procedure and actions are prescribed in the document »Ocena tveganja E-x«, stored in the folder »Z:\4-Sistem kakovosti\Zapisi\Nadzor SK\Ocena tveganja«. In the same folder we can also find Excel document »Register tveganj«, which authorizes regularly risks' and measures' changes or arrangements.

The opportunities for improvement are identified through review of the operational procedures, the policy and objectives of the quality system, internal and external audit results, risk assessment, suggestions from staff, etc. Register of opportunities are located in the second sheet of Excel document »Register tveganj«, stored in the folder »Z:\4-Sistem kakovosti\Zapisi\Nadzor SK\Ocena tveganja«.

## 2.3 Policy regarding protection of staff against improper influencing

Improper res. negative influences on the staff should be prevented by proper stimulation, good working conditions and democracy regarding determination of the quality policy.

In the case of an attempt of improper influencing a staff member should resolutely refuse any cooperation res. explains the conditions under which the laboratory is ready to cooperate. The laboratory manager should be immediately informed about every attempt of improper influencing.

## 2.4 Assurance of security of information


Customers' information that are coming from the customer or other parties (for example from a complainer or from regulators), have to be strictly confidential between the customer and the laboratory. Therefore, the laboratory staff has to keep all information, obtained and generated by laboratory's services confidential, except in the case that it is explicitly forbidden by laws. In accordance to that, all instructions regarding filing and distribution of documentation should be following precisely (see chapter 6).

Instructions regarding data transmission:

- information about calibrations is given only to the client ordering the calibrations. At the request of the client we can send the information also to the owner of the measurement equipment.
- information about calibrations is **only** sent to the client **in electronic form** (pdf document). **If they want a physical copy of the certificate, we will only issue it on request.**
- all clients' requests on information (exclusively in a written form) should be documented,
- information about calibrations can't be given by telephone.


### 3 ORGANIZATION AND MANAGEMENT

#### 3.1 Organizational structure of the Laboratory for production measurement

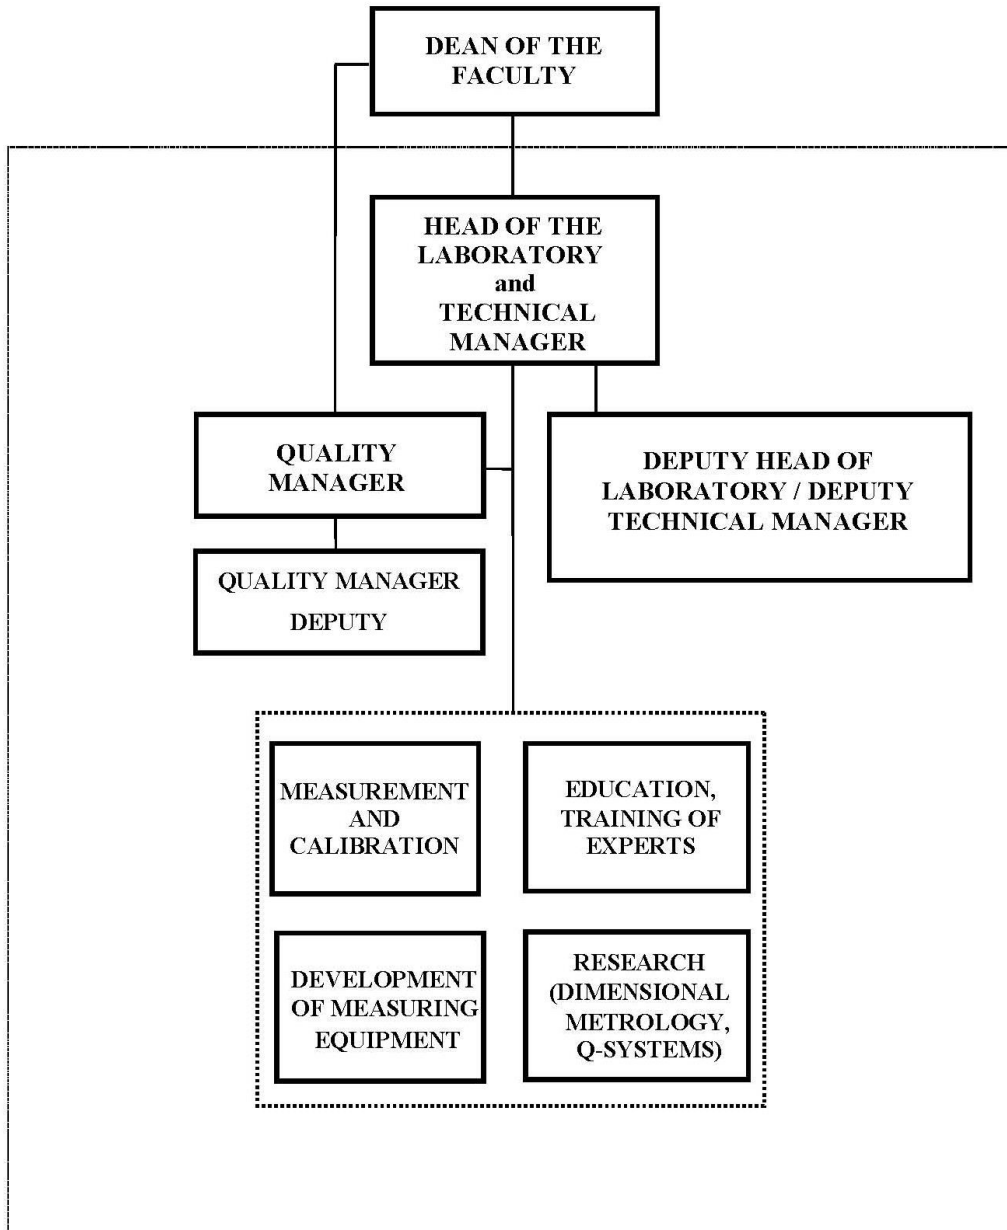

There is no hierarchical structure inside departments. Every staff member performs his work in accordance with job descriptions (P 01), defined procedures and with work instructions (Ch. 12). Certain staff members perform work in two or more departments.

Names of the leading personnel are written in chapter [3.3](#).

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>15</b> of <b>79</b>
	<b>Organization and management</b>	Issue No. <b>E-30</b>

## **3.2 Description of activities in the departments**

### **3.2.1 Department »Measurements and calibration«**


- measurements,
- calibration,
- storing and maintaining national standard of length,
- collection and update of standards,
- communication with clients,
- receipt and issue of calibration and measuring objects,
- calibration of our own measuring and inspecting devices,
- assurance of traceability of our measuring and inspecting equipment,
- maintenance of measuring and inspecting equipment,
- control of the documentation about measuring and inspecting equipment,
- creation and control of the measurements and calibration documentation,
- cooperation with the national standardization institute,
- interlaboratory comparison with domestic and foreign laboratories.

### **3.2.2 Department »Development of new measuring devices«**

- concept of measuring and inspecting devices,
- numeric analysis of measuring and inspecting devices,
- design of measuring and inspecting devices,
- manufacturing technology,
- elaboration of technical documentation,
- creation of software,
- development of system software,
- development and planning of hardware,
- development of user software,
- consulting,
- control of the documentation about the work of the department.

### **3.2.3 Department »Education, training of experts«**

- planning the education programs,
- organization of undergraduate study,
- organization of graduate study,
- performance of education (lectures, theoretical and laboratory exercises, examinations, diplomas, ....),
- work reports (to the management of the faculty),

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>16</b> of <b>79</b>
	<b>Organization and management</b>	Issue No. <b>E-30</b>

- organization of training of experts for industry,
- creation of training programs,
- performance of theoretical and practical training,
- issuing the certificates of a successfully finished training.

#### **3.2.4 Department »Research (dimensional metrology, quality assurance) «**

- research of quality assurance systems,
- research of software for CAQ,
- consulting regarding introduction of quality assurance systems according to ISO 9000,
- membership in technical committees of SMIS.
- controlling the measuring uncertainty of coordinate measuring machines (CMM),
- research in the field of measuring strategy in coordinate measuring technique,
- research of measuring software,
- research of data exchange between CAD in CMM,
- measurement and digitalization of sculptured surfaces,
- research of measuring uncertainty of the laser interferometer (LI),
- research of measuring strategy in laser interferometry,
- research of measuring software for LI,
- measurement of test measurands,
- consulting,
- control of the documentation about the work of the department.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>17</b> of <b>79</b>
	<b>Organization and management</b>	Issue No. <b>E-30</b>

### 3.3 Managers and their deputies

Rector of the University of Maribor

Prof. Dr. Zdravko Kačič

Dean of the Faculty of Mechanical Engineering:

**Prof. Dr. Matej Vesenjāk**

Principal of the Mechanical Engineering Research Institute:

**Prof. Dr. Matej Zadavec**

Leading personnel in LTM and their deputies:

Laboratory manager

(technical manager of the LTM): Prof. Dr. Bojan Ačko

Deputy Head of laboratory

(Deputy technical manager of the LTM): Dr. Rok Klobučar

Quality manager: Dr. Jasna Tompa

Quality manager deputy: Prof. Dr. Bojan Ačko

### 3.4 Management in the absence of manager(s)

The Head of the Laboratory has a deputy who was appointed on a reasoned proposal on 2 November 2021 (SK/Zapisi/Nadzor SK/Sestanki LTM: Zapisnik izrednega sestanka LTM). All activities that fall within the remit of the laboratory manager are delegated to the deputy manager for the period of his absence (e.g. signing contracts, calibration certificates, and activities relating to the quality management system ...).


### 3.5 Supervision of personnel

#### 3.5.1 Procedure for supervising the permanent personnel

The laboratory manager is responsible and authorized for the supervision of permanent personnel. The following procedure should be followed:

- daily supervision of fulfilling the work plan,
- daily supervision of the condition of the laboratory, equipment, and calibration items,
- random supervision of the performance of calibrations – whether the work instructions are followed,
- periodic laboratory meetings about current work and problems,
- check of all calibration reports and certificates issued.

Supervision of personnel by observation of the work (calibrations) performs the head of the laboratory according to the plan of observations, saved in the folder »4-Sistem kakovosti/Zapisi/Osebje/ Plan nadzora izvajalcev kalibracij.xlsx«. Short report about supervision activities and outcomes shall be entered into the plan of observations (field »Poročilo o nadzoru«).

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>18</b> of <b>79</b>
	<b>Organization and management</b>	Issue No. <b>E-30</b>

### 3.5.2 Procedure for supervising the personnel which is not yet (fully) qualified

New personnel, personnel on education, and hired personnel must be supervised in the laboratory all the time. The quality manager and the staff performing calibrations are responsible for the supervision. The following procedure should be followed:

- At least one member of the supervising staff should be always present in the laboratory.
- New personnel and personnel on education are not allowed to use the equipment used for calibrations.
- Hired personnel (which performs calibrations) is allowed to use all the equipment they need, but the first calibrations must be supervised by the supervising person and all the mistakes must be discussed and eliminated. When the supervisor decides the work is performed in accordance with the regulations and the work instructions, the supervision is not necessary any more.
- Before the new staff starts to use the work equipment, the quality manager should find out (by means of test calibrations) if the level of qualification is appropriate and if the work instructions are followed precisely.

## 3.6 Job description

Job descriptions are written in accordance with the following procedure (chapter [3.6.1](#)) and kept in P01 - »Personnel files«.

### 3.6.1 Procedure for preparing job descriptions

The laboratory management should analyze and define all the jobs res. activities necessary for the laboratory to perform in accordance with the quality policy before preparing the job descriptions.

The organizational structure res. hierarchy in the laboratory should be considered when the job descriptions are prepared.

The laboratory manager and the quality manager define all the responsibilities and authorities necessary for correct operation of the quality system.

The laboratory manager defines the authorities and the responsibilities for each member of the staff considering education, professional qualifications, experiences and the roles of individuals in the organization.


The laboratory manager defines required jobs in accordance with the organizational structure of the laboratory.

The laboratory manager assigns the jobs to the staff. The staff also cooperates with the assigning jobs. The employing conditions prescribed by the Faculty of mechanical engineering should be considered.

The laboratory manager assigns defined activities to the defined jobs. The staff also cooperates actively in this activity.

The quality manager writes the job descriptions, which include the following data:

- full name and academic title of the staff member,
- job title,
- object of the job,
- position of the job in the organization,

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>19</b> of <b>79</b>
	<b>Organization and management</b>	Issue No. <b>E-30</b>

- content of the job (activities, duties),
- necessary training, knowledge, skills, and experience,
- responsibilities,
- authority,
- reporting obligations,
- contacts (internal and external).

The job descriptions are checked and signed by the laboratory manager after he makes sure that all the staff members agree with their jobs, responsibilities and authority.

Authorized document (job descriptions) is put into the Personnel files (P 01) by the quality manager.

### **3.6.2 Procedures for amending job descriptions**

The job descriptions are amended in the following cases:

- extended activities of the laboratory,
- some defects of the existing job descriptions were detected during an internal audit,
- increased extent of work.

#### **In the case of extended activities the following procedure should be followed:**


- The laboratory manager and the quality manager define supplement activities, authorities, and responsibilities for the extended activities.
- The laboratory management organizes a laboratory meeting to analyze if a new employee is needed.
- The laboratory manager assigns new activities to the existing staff and to new employees.
- The quality manager changes the existing job descriptions.
- The amended job descriptions are checked and authorized by the laboratory manager after he makes sure that all the staff members agree with them.
- The quality manager puts the new job descriptions into the Personnel files (P 01).

#### **In the case of detected defects the following procedure should be followed:**

- The laboratory manager and the quality manager define supplement activities, authorities, and responsibilities and/or delete the existing ones.
- The laboratory management organizes a laboratory meeting to analyze if a new employee is needed.
- The laboratory manager assigns new activities to the existing staff and to new employees.
- The quality manager changes the existing job descriptions.
- The amended job descriptions are checked and authorized by the laboratory manager after he makes sure that all the staff members agree with them.
- The quality manager puts the new job descriptions into the Personnel files (P 01).

#### **In the case of increased extent of work the following procedure should be followed:**

- The laboratory management organizes a laboratory meeting to analyze if a new employee is needed.


 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>20</b> of <b>79</b>
	<b>Organization and management</b>	Issue No. <b>E-30</b>

- The laboratory manager assigns a part of the job of the person(s) with increased activities to the other staff. If the new staff is employed, new activities are prescribed for this staff.
- The quality manager changes the existing job descriptions.
- The amended job descriptions are checked and authorized by the laboratory manager after he makes sure that all the staff members agree with them.
- The quality manager puts the new job descriptions into the Personnel files (P 01).

### **3.6.3 Procedures for the case, when workers are not performing their work according to requirements**

In the case, when workers are not performing their work according to requirements (description of works, procedures...), the head of the laboratory:

- Organizes meeting with other employees and analyses the reasons of the arisen risks (e. g. insufficient technical knowledge, qualifications, and conflicts of interests...),
- After the discussion, he makes suggestions for restraining or reducing risks (like additional qualifications, motivation...),
- Follows efficiency of performed measures.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>21</b> of <b>79</b>
	<b>Quality system</b>	Issue No. <b>E-30</b>

## 4 QUALITY SYSTEM

### 4.1 Responsibilities

#### 4.1.1 Responsibility of the laboratory for quality of the work performed

The head of the laboratory takes over, in the name of the laboratory, the whole responsibility for the quality of the performed work. All possible complaints are treated in conformance with the policy and procedures describe in chapter [16](#).

#### 4.1.2 Insurance of the laboratory responsibility

Responsibility for the quality of the performed work is insured in the frame of the general insurance of the Faculty of Mechanical Engineering with a special insurance policy. The insurance premium is paid in the case when a material damage was caused to the client by the work of bad quality. In such cases the laboratory shall only analyze the justification of the complaint. The damage value is defined by the insurance company.

The height of the insurance premium is defined each year when the insurance contract is prolonged.

#### 4.1.3 Personal responsibilities


Personal responsibilities are described in the job descriptions, which are stored in Personal files - P 01. Additional responsibility descriptions can be found in the Quality manual and supporting documents for single quality system elements.

### 4.2 Quality manager


The quality manager of the laboratory is designated by the laboratory manager. His/her name is stated in Ch. [3.3](#). The quality manager is responsible and authorized for quality assurance in the laboratory. The responsibilities and authorities are listed in P01 - Personnel files. The quality manager has direct access to the Dean of the Faculty of Mechanical Engineering (Ch. [3.1](#))

### 4.3 Arrangements for permitting departures from documented policies and procedures or from standard specifications

- Departures from documented policies and procedures or from standard specifications are permitted only in unpredictable circumstances, when departures are necessary for the quality performance of the work.
- Permission for departures from documented policies and procedures or from standard specifications can be given exclusively by the laboratory manager (or by his deputy in the case of absence).
- All activities that were not performed in accordance with documented policies and procedures should be documented in the following form:
  - the name of the activity,
  - the name of the person performing the activity,
  - the date and the place of the activity,
  - the name of the equipment (if any was used),

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>22</b> of <b>79</b>
	<b>Quality system</b>	Issue No. <b>E-30</b>

- arguments for the departures from documented policies and procedures or from standard specifications,
- a list of non documented procedures used,
- a founded state about the correctness of the results of the work.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>23</b> of <b>79</b>
	<b>Documentation</b>	Issue No. <b>E-30</b>

## 5 DOCUMENTATION

Documentation of the LTM quality system is divided into the following groups:

- quality manual,
- forms for records and reports about quality system functioning,
- lists of the documents,
- standard operating procedures (SOP).


Documentation of the LTM quality system is in electronic media.

### 5.1 Location and names of the files

Valid versions of quality management system documentation are stored on the FS server ([\\fsserver.fs.um.si\LTM\\$\wp-content\uploads\2013\04](\\fsserver.fs.um.si\LTM$\wp-content\uploads\2013\04)). Links (shortcuts) of the quality manual and calibration procedures are made to the LTM web page as well as to the LTM\_lab server ([\\fsserverintranet.fs.um.si\SkupnaRaba\\$](\\fsserverintranet.fs.um.si\SkupnaRaba$)) from which laboratory staff is accessing the quality system documentation.

Folders structure is shown on the picture below.


This structure also includes databases for calibration, as well electronic records and reports (see Ch. 6).

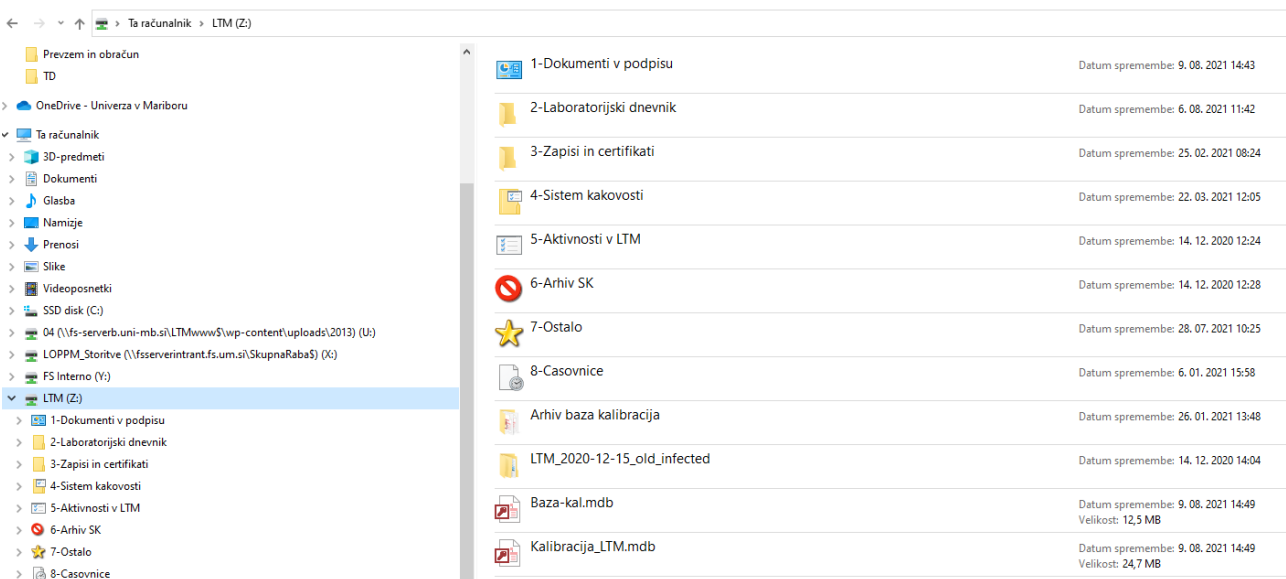

### Locations of the electronic documents and rules for naming

English versions of documents are designated with added »-en« at the end of the filename, e.g. *Poslovnik LTM-en.pdf* for the English version of the quality manual.

- quality manual: *Poslovnik LTM.pdf* – shortcut to the FS server.
- databases: *Baza-name\_of\_the\_database.mdb* – in the folder LTM (LTM server),
- forms: "Obr *mm*-title.\*", *mm* stays for the number of the form - in the folder "4-Sistem kakovosti/Obrazci",
- lists: *Title of the list.\** - in the folder "4-Sistem kakovosti/Spiski dokumentov",

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>24</b> of <b>79</b>
	<b>Documentation</b>	Issue No. <b>E-30</b>

- SOP's and their appendixes: *SOP mm.pdf* (shortcut to the FS network) and *SOP mm-priloga X.\**, mm stays for the number of the SOP, X for the name of the appendix – in the folder “4-Sistem kakovosti/ SOP”,
- records and reports about quality system: filename expresses the contents of the file with the date and/or running number, when appropriate – in the folder “4-Sistem kakovosti/Zapisi”,
- calibration certificates: *nnnn-p.pdf*, *nnnn* stays for the calibration number, -p for optional text – in the folder “Zapisi in certifikati/xxxx/Kalibracije in meritve/Zapisi in certifikati, xxxx” stays for the calibration year,
- records (about work): *nnnn\_z-p.\**, (signs meaning explained above); records are kept in the same folder as the related certificates; records are in a separate folder “Zapisi” in the corresponding SOP folder
- receipt of equipment: *client\_name-date.pdf* – in the folder “Zapisi in certifikati/xxxx/Kalibracije in meritve/Prevzem in obračun”,
- billing: *client\_name-date-spec.pdf* and *client\_name-date-račun.pdf* in the folder “Zapisi in certifikati/xxxx/Kalibracije in meritve/Prevzem in obračun”.

## 5.2 Access to the files

Access to the files in the folders, shown in the previous chapter, is limited with the system of authorized users and passwords. Head of the LTM is responsible for assigning the authorizations and passwords.

Read-only access has all personnel of the LTM and temporary staff (while working at LTM), who signed statement of confidentiality. Write access to the following folders has personnel of the LTM.

Documentation of the quality system is available for the users outside the LTM at the address <http://ltm.fs.um.si/>. Access to the quality manual is not limited, the password necessary for accessing the other documents is given to:

- Slovenian Accreditation,
- eventual other users in accordance with the laboratory manager approval.

## 5.3 Drafting, changing, approving, validity and archiving of documents

Initiative for preparing a document gives the personnel of the LTM. All documents and changes are drafted by the quality manager. Prepared documents are checked by the laboratory manager, who moves the old version to the folder *SK – arhiv* (to the filename he/she adds the issue number) and the new one to the emptied place. The laboratory manager digitally signs the document and therewith it is valid. The laboratory manager immediately informs the personnel of the LTM about the change by e-mail (or oral, if necessary) and the accreditation body by e-mail. The mail with the information shall be stored in the folder »4-Sistem kakovosti/Zapisi/Interna elektronska korespondenca«.

Documents are archived for 5 years.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>25</b> of <b>79</b>
	<b>Documentation</b>	Issue No. <b>E-30</b>

## 5.4 Protection from the use of obsolete/superseded documentation

Protection from the use of obsolete/superseded documentation (from the archive) is assured by graphical sign of archive folders and by changed filenames.

## 5.5 Rule for identification of issues

Issue number consists of the letter »E« and successive number (e.g. E-1, E-2, ...). All documents, issued before the first electronic issue of the quality manual (E-1), retain their present number until the first electronic issue.

## 5.6 Changes in the documents and new issues

At every change in the document the new document with new issue number is issued. The issue number is stated on every document page. Chapters, which were changed, added or removed, are listed in the table Evidence of changes. Changed or added text is written in the document with red colour.

Change proposals can be entered by all laboratory staff following this procedure:

- Word document (doc., oz. docx), from which the last valid (signed pdf) version was created, is moved into the subfolder »Predlogi popravkov«  
(e. g. »4-Sistem kakovosti\Poslovník\Predlogi popravkov«)
- The document name is changed by increasing the version number (e. g. document SOP 9\_E-1.doc is renamed to SOP 9\_E-2.doc)
- Document changes shall be clearly visible (red text)

When all corrections are entered, the document is reviewed by the laboratory manager, who issues the new document.

## 5.7 Procedures for protecting data from loss

Data in the folder FS.LTM5\D:\LTM are protected from loss by:

- daily backup with VEEAM on-server technology (IT FS),
- once a year back-upping of the data in the above stated folder to the digital media, which is stored by quality manager in the measurement room.

## 5.8 External documents

External documentation (official documents, standards, messages, offers etc.) is stored in the documentation file (room D 005). External documentation of LTM is divided into three groups:

- technical documentation for performance of measurements and calibrations (standards, guides, EA documents, Euromet documents, etc.),
- quality management documentation (standards like ISO/IEC 17025, guides, EA documents, SA documents, etc.),
- legal documents for the fields metrology and accreditation (law on metrology, rules, decrees, etc.)

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>26</b> of <b>79</b>
	<b>Documentation</b>	Issue No. <b>E-30</b>

- Quality manager deputy is responsible for collecting (supplementing the documentation) and up-dating the first group of documents, quality manager is responsible for the second group. The responsible persons shall review data on the web sites, standard catalogues and official gazettes (Official Gazette of Republic of Slovenia, etc.).

External documents, used for work in LTM or included in SOPs, are stated in file »Sistem kakovosti/ Spiski dokumentov /revizija.xls«. In the file also a person, responsible for checking actuality of the document and purchasing new versions, is stated. Checking of the document actuality is performed at least once a year before internal audit.

The quality manager deputy is responsible for collecting, up-dating, distributing and returning the documentation. He is also responsible for the evidence of distributed documentation (the date of distribution and the name of the person who borrows a document). Every staff member is authorized to copy the documentation for his own needs.

The valid (updated) version of a standard is always kept in the documentation file. Staff members must check the validity of their copies periodically by comparing them with the version in the documentation file.

Special documentation category is represented by contracts with SA and MIRS. These contracts define certain operating conditions of LTM. The laboratory manager is responsible for these documents. He keeps the documents in his office. One copy shall be available to the dean of the Faculty of Mechanical Engineering.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>27</b> of <b>79</b>
	<b>Reports and records</b>	Issue No. <b>E-30</b>

## 6 REPORTS AND RECORDS

### 6.1 Reports

Performer of the calibration writes a report, converts it in pdf file and submits it to the authorized person for digital signing. Signed version is saved in the pdf format (see Ch. 5). **The report is sent to the customer by e-mail or, at the customer's request, printed out and sent to the customer together with the measuring device(s).**

#### 6.1.1 Calibration reports

The first page of a calibration report is created from the database »Kalibracija\_LTM.mdb«, which is stored in the folder LTM (LTM server). Instruction for entering data is in the folder »2-Laboratorijski dnevnik«.

The second and the subsequent pages of the certificate are created from the templates, which are stored in folders of corresponding calibration procedures (»4-Sistem kakovosti/SOP/SOPX«). The list of templates (for individual SOP's) which are used for creating records and other pages of certificates are stored in the folder »Sistem kakovosti/SOP/Sledljivost predlog po SOP-ih.xlsx«. Accredited and non-accredited certificates are created by using the same templates. In the case of an accredited activity, the accreditation mark (SA) in the templates is clearly marked with a red border (Word templates) or using the button »Accredited certificate« (Excel templates). The same applies to the CIPM MRA logo. In the case of issuing a non-accredited certificate from Word templates, both logos shall be removed. In accredited certificate, the red border shall be removed. A detailed description of the scope of accreditation (SA and CIPM) is in the document »Obseg akreditacije SA in CIPM.docx« in the folder »2-Laboratorijski dnevnik«.

#### 6.1.2 Instructions for amending/supplementing reports

- If it is necessary to change a report/certificate after it has been issued, a completely new document should be written.
- The new issue number of the certificate consists of the letter (e.g. A, B, C...) and the number of the certificate already issued. For example, the number of the certificate: 12111-LTM-22; thus, the first supplement to the report would consist of a letter »A« (second supplement »B«, third »C«, etc.) and the number 12111-LTM-22, i.e., A12111-LTM-22.
- Corrections/supplements to the document must be clearly marked with an asterisk (\*).
- A new issued document must contain an original reference in a remark.
- All holders of the original report/certificate should get the corrected (new) report/certificate.
- The corrected (new) report/certificate should be filed together with the original report/certificate.

#### 6.1.3 Instructions for distributing copies of the records

When the client demands a copy of the record (e.g. after losing it), **we will send it to him by e-mail or, at his request, we will print out the report from the \*.pdf file and send it by post.**

### 6.2 Records

There are paper and electronic records. Rules for handling with electronic records are stated in Ch. 5.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>28</b> of <b>79</b>
	<b>Reports and records</b>	Issue No. <b>E-30</b>

### 6.2.1 List of records

The following records should be filed in the laboratory:

- Records on performing calibrations, which should contain sufficient data for repeating the calibration any time. The records are most often created from templates (Predloga\_zapis-SOPX) which are stored in the folder »4-Sistem kakovosti/SOP/SOPX«. These records are stored in electronic form - pdf files (see Chapter 5.1). Each electronic record of calibration performance must be digitally signed (**identity, date**).

Paper records can be scanned to pdf file immediately after they are finished, and therefore related as electronic records (see Ch. 5.1). When a paper record is not scanned, it must be stored, as stated the calibration procedure – SOP (Chapter: Documentation).

- Records of supplies and services, which should contain:
  - report about the assessment of suppliers,
  - purchasing documentation,
  - report about the inspection (tests) of the incoming goods,
  - suppliers' information about the quality of the products.

Paper records are stored in the Z 02, electronic in the folder »4-Sistem kakovosti\Zapisi\OPREMA«.

- Records about the quality system (internal audits, external assessments, management reviews, non-conformities, corrective actions etc.): paper records in Z 04, electronic in »4-Sistem kakovosti\Zapisi\Nadzor SK«,
- Records about subcontracting (Z 06),
- Records about complaints and related actions: electronic in »2-Laboratorijski dnevnik/ Register pritožb«,
- Records about the environmental conditions in the laboratory: electronic in »4-Sistem kakovosti\Zapisi\OPREMA«,
- Statements and Authorizations: paper records in Z 09, electronic in »4-Sistem kakovosti\Zapisi\Izjave in pooblastila«,
- Records about calibration software validation: electronic records in folder »4-Sistem kakovosti\Zapisi\ Validacija programske opreme«,
- Personal file (P 01), paper records in P 01, electronic in »4-Sistem kakovosti\Zapisi\OSEBJE«,
- Equipment file: paper records in E 01, electronic in »4-Sistem kakovosti\Zapisi\OPREMA«.

### 6.2.2 Indexing, storage and archiving records on paper

- Each record should carry the serial number and the date.
- The records are arranged by serial numbers (and also by dates).
- All valid records for current year are stored in the documentation file in the room D 005.
- All records, stated in previous chapter, are to be archived for 5 years in the room D 004. After elapsing that time records are to be destroyed – cut in pieces and disposed.
- The quality manager is responsible for indexing, storage and archiving of records on paper.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>29</b> of <b>79</b>
	<b>Reports and records</b>	Issue No. <b>E-30</b>

### **6.2.3 Indexing, storage and archiving of electronic records**


- Record (computer files) which are not defined in ch. 5.1 are named in a way that the name describes the record, date, year and consecutive number are added, when suitable. Storage is described above.
- Elektronic records are archived in the folder Arhiv SK in the corresponding subfolder for 5 years.

### **6.2.4 Procedure for lending out the filed records**

- The quality manager deputy is responsible for lending out and for returning the documents.
- The original records on paper can be lent to all staff performing calibrations, but they should not be delivered out of the laboratory. The records can be copied only by request of the client, the subcontractor, and the accreditation body.
- Electronic records are not to be printed, with exceptions of the cases in the paragraph above.
- The copies of the records cannot be distributed, except to the accreditation body (which can get all records), to the client (who can get only the records related to the calibration of their items), and to the subcontractor (who can get the records of calibrations performed by them).
- and authorized to decide who can get the copies of the records.
- Clients and subcontractors can get copies of records only by sending us a written (official) request. Copies are sent as a registered mail in order to get a clients' confirmation of receipt.
- When a document is returned, the authorized person should check if the document is complete (the number of pages compared with the number on the lending out note).

### **6.2.5 Guidelines for changing records**

- A record can be changed (corrected) only during the creation, if a writing error has been detected. When a record is filed res. put in a folder, it is not allowed to be changed any more. This rule concerns paper and computer records.
- If certain part of a record has to be changed, incorrect text shall be crossed out (not erased or darkened) and the correction shall be signed by the person, who has written (and also corrected) the record.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>30</b> of <b>79</b>
	<b>Quality system control</b>	Issue No. <b>E-30</b>

## 7 QUALITY SYSTEM CONTROL

### 7.1 Internal quality audits

#### 7.1.1 Guidelines for performing internal quality audits

- Internal quality audits are planned, organized and documented by quality manager.
- Internal quality audits are performed by a group composed of the head of the LTM and quality manager.

#### 7.1.2 Planning of the internal quality audits

Periodical (regular) internal quality audits are performed once in a year. Quality manager informs in time the LTM personnel and audit performers by e-mail. Audit of performance of calibration on site is defined in Ch. 13.6.1.

#### 7.1.3 Instructions/checklists for performing audits

The person who audits components of the quality system should use the form »Obr 11-Spisek preverjanj int.presoje v lab.doc«, stored in the folder »Obrazci« (see Ch. 5.1).

#### 7.1.4 Audit report

Audit report is to be written on the form »Obr 09-Poročilo o interni presoji.doc«, stored in the folder Obrazci (see Ch. 5.1). Reports are digitally signed and named »4-Sistem kakovosti\Zapisi\Nadzor SK\Interne presoje\LLLL\Poročilo o interni presoji X-LL.pdf«. A report number consists of running number (X) and year (LL): X-LL.


#### 7.1.5 Nonconformance and corrective actions

Ascertained non-conformances are written in file Neskladnosti in kor.ukrepi.xls in the folder »4-Sistem kakovosti/Zapisi/Nadzor SK«. Also proposed corrective actions and checking are written in this file. When all corrective actions are checked and approved by head of the LTM, he adds the date in the column »Preverjeno«.

### 7.2 Management review

Management reviews are to be performed using the next procedure:

- Review is carried out once a year after the internal audit,
- Review is conducted by the laboratory manager,
- Review shall be attended by the entire laboratory staff
- Review should include at least the following items:
  - matters arising from the previous review,
  - reports on surveillance and re-assessment visits carried out by any accreditation body,
  - results of internal audits carried out since the last review,
  - analysis (execution and efficiency) of corrective and preventive actions,
  - efficiency analysis in the case of performed risk and opportunities measures,

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>31</b> of <b>79</b>
	<b>Quality system control</b>	Issue No. <b>E-30</b>

- results of the laboratory's participation in any proficiency testing or interlaboratory comparison schemes and the need for such participation in other areas of calibration,
  - results of any in-house quality control checks,
  - up-dating quality risks, detecting changes that can affect quality management,
  - details of any complaints received from customers,
  - need for amendment of the quality system, including the quality manual,
  - need for amendment or updating a price list of calibrations and other services,
  - achieving of quality objectives,
  - plan for the implementation of decided changes to the quality system, including a timetable,
  - adequacy of current human and equipment resources,
  - future plans and estimates for new work, additional staff, new equipment etc.,
  - training of new staff and updating of existing staff,
- A record should be written after each review using the form »Obr 08-Zapisnik vodstvenega pregleda.doc«, stored in the folder **Obrazci** (see Ch. 5.1). Report is saved as \*.pdf and digitally signed.
- The quality manager is responsible for the control of the performance of activities defined at the review.

## **7.3 Quality system control during the work**

### **7.3.1 Procedures for reporting and registering nonconformities**


After finding a nonconformity or equipment defect in a part of the quality system, a person, responsible for this part of the system, shall immediately inform the head of the laboratory, who enters the nonconformity into the document »Neskladnosti in kor.ukrepi.xls« in the folder »4-Sistem kakovosti/Zapisi/Nadzor SK« (same procedure as in internal audit). Data about a nonconformity shall include at least the following:

- name of the person, who registered the nonconformity,
- date and location of the nonconformity registration,
- type of the nonconformity,
- name and identification of defected equipment (if any),
- the circumstances at the registration of the nonconformity,
- the expected influence on the calibration results.

### **7.3.2 Procedures for execution of corrective actions**

Instructions for correcting the nonconformities are given from the quality manager after examining the nonconformities report and analysis for appearance of nonconformities (procedure for analyzing in Ch.7.3.3). The nonconformity is to be corrected by a person, responsible for a part of the quality system where nonconformity has appeared. Instructions given from the quality manager are to be precisely followed.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>32</b> of <b>79</b>
	<b>Quality system control</b>	Issue No. <b>E-30</b>

Report about executing a corrective action shall be entered into the column »Opis izvedenega« in the document »Neskladnosti in kor.ukrepi.xls«.

Corrective action is checked by the head of the LTM.

### **7.3.3 Procedure for analysing deficiencies, complaints etc. and for investigating their causes**

The analysis of deficiencies, complaints etc. and the investigation of their causes is performed by the quality manager.

A person who detected a non-conformity and is responsible for the part of the quality system where the non-conformity appeared, cooperates in the analysis.

The analysis is performed in the following steps:

- historical examination of the quality system element containing deficiency resp. defective equipment (have some deficiencies or defects occurred before?),
- which personnel is involved,
- consideration whether the deficiency res. the defect occurred because the quality policy had not been respected,
- searching for causes (objective, personal),
- analysis of the deficiency influence on the operation of the quality system,
- analysis of the deficiency influence on the calibration results,

The quality manager makes conclusions of the analysis and investigation and proposes corrective actions in order to eliminate deficiency and the causes for deficiencies.

The quality manager writes an investigation report, which includes conclusions and proposed corrective actions. The report is given to the laboratory manager, who approves (or rejects) the proposed corrective actions. Report is saved as \*.pdf and digitally signed.

### **7.3.4 Procedure for checking whether work is required to be either wholly or partially redone**

The quality manager deputy checks calibration records in order to find out which (if any) were performed in the time when the deficiency or equipment defect was present. After that possible influence of the deficiency on the calibration results are defined using the investigation report (Ch. 7.3.3). Data about the calibrations that are suspected to be irregular are given to the quality manager.


The quality manager informs the clients about the possibility of irregular calibration results by phone. Written explanation including the causes for irregular results is sent to the clients as well.

The laboratory manager decides whether work is required to be either wholly or partially redone. This decision is based on the deficiency analysis and investigation report. The quality manager and the calibration staff are also involved in this decision. If certain calibration is required to be redone, the calibration staff and the client are informed by the laboratory manager.

The repeated calibration should be included into the work plan. However, the schedule for other calibrations must not be changed and client's requirements must be considered. The calibration must be repeated after the regular working time if necessary.


The results of the repeated calibration must be reported to the quality manager and the laboratory manager.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>33</b> of <b>79</b>
	<b>Quality system control</b>	Issue No. <b>E-30</b>

The quality manager checks the results of the original and the repeated calibrations and writes conclusions about the validity of the original calibrations. These conclusions should be filed into the register of corrective actions. All records of invalid calibrations should be marked with “INVALID” and filed into a separate folder.

After the quality manager has written the conclusions about the validity of the original (first) calibration, he should send a report to the client. The results of the repeated calibration should be included in this report.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>34</b> of <b>79</b>
	<b>Personnel</b>	Issue No. <b>E-30</b>

## 8 PERSONNEL


### 8.1 Policy regarding the personnel performing calibrations

- Personnel performing calibrations shall be properly qualified. Requirements regarding formal education, technical knowledge and experiences are defined in chapter 8.2.1 and in job descriptions (P 01), whether the requirements regarding periodical education are in chapters 8.3.1 and 8.3.3;
- Proper supervision for not yet fully qualified personnel and for personnel in education process shall be assured in accordance with the procedure 3.5.2;
- In the case of hiring personnel we shall properly define requirements, supervision and qualification of such personnel. The procedure 8.2.2 shall be followed;
- Unique job descriptions shall be available for all employees according to the procedures 3.6.1 and 3.6.2;
- Personnel performing calibrations shall be authorized by the laboratory manager. Authorizations are collected in the document »Matrika pooblastil.pdf« in the folder »4-Sistem kakovosti/zapisi/osebje/pooblastila«. Reference to this document is stated in the job descriptions (P 01). Authorizations for using equipment are listed in chapter 10.4 and in job descriptions (P 01). Hired personnel shall get a written authorization from the laboratory manager before performing any kind of work in calibration field.

### 8.2 Selection and recruitment

#### 8.2.1 Procedure for recruiting and selecting personnel

- The laboratory manager is authorized and responsible for recruiting and selecting personnel.
- The laboratory manager decides to employ new personnel when the work extent increases, a worker leaves certain working position or a worker is moved to another working position.
- The decision about employing new personnel is reported to the authorized body of the Faculty of mechanical engineering, which brings an official decision about employing new personnel and advertises a vacancy.
- New personnel must meet all the requirements (education, knowledge, skills, and experiences) defined in job descriptions (Personnel files P 01).
- When selecting a new worker among all the candidates who meet the requirements, the level of education, skills, and experiences should be considered in the following order:
  - level of education,
  - working experiences in the field of dimensional metrology,
  - physical skills (for the personnel performing calibrations),
  - knowledge and experiences in the field of quality systems,
  - results res. quality of the past work.
- A new worker is employed in accordance with the UM-FS rules (normally for limited period of 1 year). Activities in the fields of calibration for clients can not be started until the new worker is authorised by the laboratory manager. The authorization is based on successfully

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>35</b> of <b>79</b>
	<b>Personnel</b>	Issue No. <b>E-30</b>

concluded training (procedure in [8.3.1](#)). During the training period, the new worker is supervised by a staff member responsible for the field in which the new worker was employed (see also [3.5.2](#))


### **8.2.2 Procedure for hiring temporary personnel**

- The laboratory manager is authorized and responsible for hiring temporary personnel.
- Temporary personnel is hired exclusively for calibration.
- The laboratory manager decides to hire temporary personnel when the work extent increases or when a permanent staff member is absent for a period longer than six months because of illness, education, training, etc.
- The laboratory manager writes the contract (by the help of the lawyer at the Faculty of mechanical engineering), which should be signed by a hired person and the laboratory manager. The agreement of the Faculty of mechanical engineering is not required.
- The hired person must meet all the requirements (education, knowledge, skills, and experiences) defined in job descriptions (Personnel files P 01).
- When selecting a worker among all the candidates who meet the requirements, the level of education, skills, and experiences should be considered in the following order:
  - working experiences in the field of dimensional metrology,
  - results res. quality of the past work (known from the cooperation in the past),
  - physical skills (sight, concentration, ...),
  - level of education,
  - knowledge and experiences in the field of quality systems,
- Hired person should perform test calibrations (typical examples) under supervision of the permanent staff (an authorized staff member). The supervising person evaluates the work and decides whether the hired person is able to work correctly or not.

## **8.3 Education**

### **8.3.1 Procedure for training new staff**

- The laboratory manager is responsible and authorized for planning the training and for proving staff qualifications and competence.
- Immediately after employing a new staff member, the laboratory manager defines a strategy of including him in the service activities of the laboratory and prepares a training plan. (stored in the folder »4-Sistem kakovosti/Zapisi/Osebjje/Plan usposabljanj za nove dejavnosti in ljudi«). Performers, necessary time consumption and dates of education are defined in the plan.
- When the performers of education confirm that the new employee is fully competent for performing certain activity, the laboratory manager writes a training report (electronic document in the folder »4-Sistem kakovosti/Zapisi/Osebjje/Poročila o usposabljanju/let«), which also includes authorization for performing certain service activity. The document is printed and signed. After that it is filed in the folder P 01.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>36</b> of <b>79</b>
	<b>Personnel</b>	Issue No. <b>E-30</b>

- When the training report (with authorization) is issued and authorised, the laboratory manager updates the document »4-Sistem kakovosti/Zapisi/Pooblastila/Matrika pooblastil.« This document is signed and filed only in electronic form.


### 8.3.2 Procedure regarding the periodic checks of staff qualification

- The laboratory manager is responsible for the periodic check of staff qualification.
- The periodic check of qualification of the management staff is ensured by increasing education level to doctor's degree (internal check) and after that by working on professional projects and by publishing in professional magazines, proceedings etc. (external check).
- The qualification of the staff performing calibrations is checked by the management staff once a year. The following items are checked:
  - completed professional training in the check period,
  - working methods (comparison with the methods used in other accredited laboratories),
  - optimal use of computers for calculation and transfer of measuring data.

The periodic qualification check is a part of the quality system audit.

### 8.3.3 Description of the training system

- The training is divided to:
  - regular (periodic) training, which assures that the knowledge level of the personnel follows the development in the field of their work,
  - special training in the cases of buying new equipment, extending the field of work, changing the measuring and calibration methods, etc.
- The staff is required to train periodically in the following ways:
  - following and ordering new editions of important professional literature and informing the colleges,
  - getting information about the newest professional literature available in libraries, by international library cooperation, and by order,
  - visiting important metrological fairs. Every staff member should visit at least one domestic fair per year and one international fair every two years,
  - attending conferences, workshops, etc. The staff with the 7th degree of education is obliged to send their contributions to at least two conferences a year,
- If some special training is necessary, the laboratory manager consults the quality manager and the staff performing calibrations and brings the decision about the organization of the training.
- Special training can be performed in the following ways:
  - training for the use of new equipment (training at the manufacturer, practical training in the laboratory, study of the supporting literature, guides etc.). Training at the manufacturer and/or training in the laboratory must be attended by all the staff members who will work with the new equipment. Other staff members should be informed by the trained staff about the purpose, applicability, and operating principles of the new equipment,
  - attendance at selected conferences and fairs (new measuring methods, new measuring equipment, ...),

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>37</b> of <b>79</b>
	<b>Personnel</b>	Issue No. <b>E-30</b>

- study of a selected new literature (new standards, work instructions, legal requirements, work methods, ...),
- studying at other universities and institutes.
- The laboratory manager is responsible and authorized for the preparation of the program for special training and for financial realization.
- After the training the staff member should write a training report (Obr 25), in which he shall give his opinion on training effectiveness. The laboratory manager supplements the report with his evaluation of the usefulness and success of the training. A certificate of a successfully finished training (if it is granted) shall be attached to the training report. Training reports are analysed on management review.
- All certificates of a successfully finished training, training reports, and laboratory manager evaluations should be included in the personal files.

## **8.4 Documentation**

### **8.4.1 Instructions on keeping the personal files**

- Complete personal documentation (with the exception of certificates regarding periodic and special training) is filed at the personnel department of the Faculty of mechanical engineering.
- The copies of the personal documentation are filed in the documentation file in the room D 005.
- The personal file is marked with the code P 01.
- The rules regarding filing, protection, lending and copying are the same as in the Ch.6.2.2.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>38</b> of <b>79</b>
	<b>Facilities</b>	Issue No. <b>E-30</b>

## 9 FACILITIES

### 9.1 Using the special installations

#### 9.1.1 Operating instructions for special installations

There are three special installations in the laboratory - air conditioner for measuring rooms, air conditioner for the air-conditioned chamber and the air compressor.

##### 9.1.1.1 Air conditioner

- the air conditioner is adjusted and maintained exclusively by the authorized service,
- if a staff member detects disturbances in the operation of the air conditioner (disallowed temperature deviations), he (she) should inform the quality manager deputy, who is authorized and responsible for contacts with the authorized service.

##### 9.1.1.2 Air conditioner for the air-conditioned chamber

- the authority for adjusting parameters of the air conditioner is assigned to the same personnel as the authority for using calibration equipment (chapter 10.4.1),
- parameters can be changed only in cases of special measurements and disallowed deviations from required climatic conditions in the chamber,
- the original manufacturer's (IZR) user's guide should be used for changing parameters, the guide is available in the chamber,
- all parameter changes should be recorded **with the ALMEMO measuring system**,
- if a staff member detects disturbances in the operation of the air conditioner (disallowed temperature deviations), he (she) should inform the quality manager deputy, who is authorized and responsible for contacts with the authorized service.

##### 9.1.1.3 Air compressor

- when the compressor is not in use, it is turned on, but the air valve must be closed,
- the compressor is activated by opening the valve on the output pipe,
- the condensed water should be eliminated from the compressor by opening the valve under the output pipe before using the compressed air.

### 9.2 Access and use of spaces and installations

#### 9.2.1 Access to the spaces and installations

- all permanent staff members have an access to the measuring and the office rooms,
- the staff performing calibrations, the laboratory manager, and the quality manager have access to the room with the air conditioner and the air compressor,
- unlimited access to the climatic chamber is assigned to the same personnel as the authority for using calibration equipment (10.4.1),

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>39</b> of <b>79</b>
	<b>Facilities</b>	Issue No. <b>E-30</b>

- other laboratory members are allowed to enter the climatic chamber under supervision of the authorized personnel,
- persons, who are not employed in the laboratory, are not allowed to enter the climatic chamber (exceptions are special occasions like services, installation of equipment etc. - in these cases entrance should be allowed by the laboratory manager and persons entering the laboratory should be supervised by at least one authorized person),
- other installations are available to all staff members.

### **9.2.2 Instructions for the use of spaces**

- all permanent staff members have keys of all laboratory rooms,
- a staff member can get new res. spare keys only with the agreement of the laboratory manager,
- the keys must not be lent to the people who are not employed in the laboratory,
- people who do not work in the laboratory can enter the rooms only in the presence of a staff member,
- temporary laboratory staff can get the keys, but they must sign a statement in which they confirm an agreement with the laboratory quality policy,
- when a staff member leaves a laboratory room, he (she) must close the door, which is then automatically locked. After the working time the doors must be additionally locked,
- when entering or leaving the measuring room only one door can be opened at the time (the glass door can be opened after the main door has been closed or vice versa),
- staff should wear white coats in the measuring rooms,
- in the separation room the shoes must be cleaned and the upper clothes (coats etc.) must be changed with a white coat,
- smoking is forbidden in all rooms,
- furniture and measuring equipment (except handy measuring devices) can be moved only with the agreement of the laboratory manager. All changes should be updated in the laboratory plan,
- for climatic chamber we should apply the same rules as for other spaces (except the rules regarding access to the spaces and the possession of keys), and the following three additional rules,
- climatic chamber should be locked when the authorized personnel is absent,
- only personnel performing calibrations have keys of the climatic chamber,
- the climatic chamber is cleaned by the personnel performing calibrations (cleaning personnel has no right to enter the chamber).

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>40</b> of <b>79</b>
	<b>Facilities</b>	Issue No. <b>E-30</b>

### **9.3 Climatic conditions in the laboratory**

#### **9.3.1 Reference conditions**

Specified reference conditions in rooms D1 004 in D1 005 concern only temperature and humidity. The temperature shall be  $(20 \pm 1)$  °C, while the recommended relative humidity is  $(50 \pm 20)$  %.

In the microclimatic chamber at the working height (approx. 80 cm) the temperature shall be in the range of  $(20 \pm 0,1)$  °C, while the recommended relative humidity is  $(50 \pm 20)$  %.

#### **9.3.2 Registering conditions**

Combined instrument Belmont for registering temperature, humidity and pressure is used for registering climatic conditions in all rooms. System is adjusted to register data every 15 minutes. Every month the data for the current month is transferred on the LTM server (»Sistem kakovosti/Zapisi/Pogoji v laboratoriju/LLLLMM.xls«). Complete measurement data is kept in the Almemo system until the memory is full. After that the whole data package is transferred on the LTM server.

The instruction of using measurement-registering device Almemo is in the folder »Sistem kakovosti/Delovna navodila«.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>41</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

## 10 EQUIPMENT

### 10.1 Policy for achieving traceability of measurements

- All calibrations shall be traceable to a primary (international) standard of measurement.
- Every new measuring device must be calibrated before the first use.
- All measuring devices and standards used for calibrations shall be calibrated in the defined calibration intervals (**document »Plan kalibracij.xls«**).
- Measuring devices and work standards are calibrated in the laboratory. Calibrations shall be performed in accordance with the instructions in 10.7 and in SOP.
- Reference standards of measurement are calibrated in selected accredited or national laboratories by primary standards or by standards that were calibrated directly by primary standards.
- Calibrations shall be documented (instructions in 10.7). **The calibration documentation should be stored on the server and partially** in the records of the equipment (E 01).
- The user of equipment can check the status of traceability (valid calibration) in the document »Plan kalibracij.xls« in the folder »2-Laboratorijski dnevnik«.
- The quality manager deputy is responsible for regular and correct calibration and for calibration documentation.
- Indicators are used to control quantities with influence on the measurement (e.g. environmental conditions). Correctness of the indicator is checked with appropriate calibrated measure in the time interval, as stated in the evidence sheet.

### 10.2 Identification and evidence

#### 10.2.1 Equipment file

##### 10.2.1.1 List of capital goods (equipment of greater value)

- A list of basic means of the Laboratory (expense account No. 2101) is filed and maintained on the level of the Faculty (controlled by bookkeeping department). It is also filed in the Computer center of the University in Maribor.
- The list contains:
  - inventory number,
  - name of equipment,
  - status,
  - real and write off value,
  - begin of the balance,
  - amortization and revalorization group,
  - account,
  - location

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>42</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

- A new basic good (equipment) is accepted by a protocol that is signed by:
  - the Dean of the Faculty,
  - the laboratory manager,
  - designated user of the equipment.
- An inventory number is attached to the equipment.
- A copy of the list of basic goods is filed in the folder Equipment files (E 01), filed in the documentation file in the room D1 005.

#### 10.2.1.2 Evidence sheet

- Traceable measuring devices are registered on evidence sheets.
- A field of evidence contains:
  - name of a device,
  - measuring range,
  - resolution,
  - evidence number (inventory number),
  - owner,
  - manufacturer,
  - manufacturers' identification,
  - date (year) of manufacture,
  - classification,
  - term of periodic calibration (legal or intern),
  - date of first calibration,
  - performer of first calibration,
  - approval of the laboratory manager for the use of new equipment (signature)
- A field of periodic calibration contains:
  - serial number,
  - date of calibration
  - performer(s) of calibrations,
  - identification of a certificate,
  - person(s) who approved calibrations,
  - notes.
- Evidence sheets are issued by the user in the laboratory. The sheets are based on the protocol of acceptance.
- The evidence sheets are saved on the LTM server »Z:\4-Sistem kakovosti\Zapisi\OPREMA\Evidenca in status opreme«.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>43</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

### 10.2.2 Identification of measuring equipment

- The entire equipment is identified by inventory numbers. They are printed on metal or plastic plates that are attached to the equipment.
- Most of measurement instruments and other equipment are also identified by serial res. Factory number. This identification is used in cases, when inventory numbers are not available (e. g. more components under same inventory number).
- Calibration status is identified with calibration sticker (same as for clients), which contains the date of the last calibration. The date of the next calibration can be found in the evidence sheet as well as in the electronic record »2-Laboratorijski dnevnik/Plan kalibracij.xls«.

### 10.2.3 Instructions for keeping the equipment files

- The following equipment files are kept in the laboratory:
  - documents about authorization for using the equipment,
  - documents about the equipment used for calibration,
  - documents about the equipment used for measurement.

## 10.3 Issue and receipt

### 10.3.1 Procedures for supervision, issue and receipt of equipment

- Only manual measuring equipment that is not used for calibration (accredited or non-accredited) is allowed to be lent out,
- Equipment, which is lent (or brought) outside the laboratory, must be registered. A bond, issued for the issued equipment, should contain the following information:
  - address of the Laboratory for production measurement,
  - address and telephone number of the institution borrowing the equipment (if it is lent out),
  - location of the equipment during the period, when it is outside the laboratory,
  - bond number,
  - number of pieces of the equipment (if the equipment, carrying one inventory number, contains more parts, all parts must be quoted),
  - name of the equipment,
  - manufacture and inventory number,
  - date of issue, lending period, date of return,
  - name and signature of the person issuing (receiving) the equipment,
  - name and signature of the person borrowing (returning) the equipment.
- The bond is issued in two copies. The original is kept by the laboratory, whereas the second copy is given to the institution (person) borrowing the equipment.
- Bonds of issued and returned equipment are filed in the folder E 01, **located in the document department in room D1 005.**

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>44</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

- At the time of return the equipment must be checked (function and damages). When needed, precise equipment must be calibrated after return.
- Issue of equipment must be approved by the laboratory manager.

### 10.3.2 Rules for borrowing equipment from third parties

- We borrow only missing equipment for calibration and measurement. If borrowed equipment is not traceable, it is calibrated in the laboratory in accordance with the laboratory authorities.
- Bonds of borrowed equipment are filed in the folder E 01, **located in the document department in room D1 005.**

## 10.4 Authority

### 10.4.1 Rules regarding the authority to use the equipment

- Calibration equipment may be used only by properly qualified staff members.
- The following staff members are authorized for using the calibration equipment:
  - Bojan Ačko,
  - Lucija Črepinšek Lipuš (with limitations, see personal map),
  - Mitja Mlakar (with limitations, see personal map),
  - Rok Klobučar (with limitations, see personal map),
  - Jasna Tompa (with limitations, see personal map).
- Other persons can use the equipment only by special authorization of the laboratory manager. The authorization for the use of the equipment contains:
  - address of the laboratory,
  - authorization number,
  - list of equipment,
  - manufacture and inventory numbers,
  - period of authorized use of equipment,
  - name and signature of the user,
  - signature of the laboratory manager.
- The authorization is issued in two copies. The original is filed in the folder E 01, whereas the copy is given to the user.

## 10.5 Equipment locations

All laboratory equipment is located in rooms D1 005 and D1 004. In D1 005 we have the Coordinate measuring machine, gauge block comparator and some manual equipment. All other equipment is located in room D1 004. The equipment of the highest metrological level is located in the microclimatic chamber in room D1 004 (exception is the primary standard – frequency stabilised laser, which represents the highest metrological level; since environmental condition limitations are not very strict, it is located outside microclimatic chamber).

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>45</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

## 10.6 Maintenance

### 10.6.1 Maintenance instructions

- The original instructions of manufacturers should be used for the maintenance of the equipment.
- Service periods are based on the recommendations of manufacturers. Repairs should be performed only by authorized services.
- Maintenance plans and addresses of authorized services are kept in the folder E 01.

### 10.6.2 Lists of spare parts

- Lists of spare parts are kept in the folder E 01.

## 10.7 Calibration

### 10.7.1 Procedures for calibration of the equipment

- A procedure for the calibration in the laboratory:
  - all measuring instruments and work standards are calibrated in the laboratory,
  - calibration should be performed in accordance with calibration procedures (Ch. 12.4) and work instructions,
  - calibration reports and certificates should be saved on the LTM server in folders »Z:\4-Sistem kakovosti\Zapisi\ OPREMA\Evidenca in status opreme«,
  - dates of calibration should be noted on evidence sheets.
- A procedure for calibration outside the laboratory:
  - reference standards and other equipment used for assuring traceability of measurements and calibrations, which can not be calibrated in the laboratory, are calibrated in other institutions;
  - the head of the laboratory is responsible for choosing calibration laboratory;
  - the offers are collected by the quality manager and his deputy in accordance with procedures in Ch. 11;
  - the most important criterion for selecting a laboratory is its best calibration capability;
  - quality manager is responsible for the communication with calibration laboratories;
  - an order for calibration shall include the form of calibration results, the limits of measuring uncertainty, the period of calibration and reference to the order price;
  - quality manager is responsible for the transportation of the equipment. The transport is organized by the office (on the faculty level) which is co-operating with a forwarding agency (this agency also organizes the transportation);
  - suitable package shall be available for all standards and other equipment. Quality manager deputy is responsible for marking the package with all necessary data for transport (addresses, instruction for handling);

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>46</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

- when the equipment is returned from calibration, the user (the one who is in charge for it) shall check if and write a short record if significant changes are detected. The changes are analyzed by the quality manager and a warranty procedure is initiated if necessary.

### 10.7.2 Program for performing periodic calibrations

A register of equipment and calibration intervals are written in the folder E 01. Recalibration intervals are defined by the laboratory manager. Professional judgement is based on the expertise and the history of measurement instruments and standards. Changes in recalibration intervals are decided and confirmed by the laboratory manager by entering new interval in the evidence sheets. New entry shall be confirmed by date and signature. After a new change is confirmed, the quality manager updates the electronic document »4-Sistem kakovosti/Laboratorijski dnevnik/Plan kalibracij.xls«.

### 10.7.3 Analysis of calibration results

Results shall be analysed after each calibration (in LTM or outside) according to the following procedure:

- the results from the last certificate are compared with the results on previous certificate(s).
- calculate factor  $E_n$ , the satisfactory value is less than 1

$$E_n = \left| \frac{\text{rezultat}_2 - \text{rezultat}_1}{\sqrt{U_1^2 + U_2^2}} \right|$$

- if the deviations are in limits of specified uncertainty res it is found out that they do not increase the uncertainty of calibration or measurement for which the equipment is used, the head of the laboratory approves the use with a signature in the field »Periodic calibration« of the evidence sheet,
- if detected deviations could threaten trust in calibrations pr measurements for which the equipment is used, the technical commission (head of the laboratory, quality manager and a user of the equipment) analyses causes for such deviation(s) and checks a possibility that calibrations, which have already been performed, are not confident. I necessary, such calibrations are repeated,
- if causes cannot be detected by the analysis, the equipment is recalibrated (if possible in other institution),
- a report of the analysis (including all conclusions) is written and save into the folder »4-Sistem kakovosti\Zapisi\OPREMA\Poročila o analizi kalibracij«,
- a »history« of equipment in a for of comparison table or graphs is managed for reference standards (in the folder »7-Ostalo\LTM-delo-izobrazevanja-organizacija-splet-projekti\Baza kalibracij-narocniki«)
- if it is necessary to change calibration values of a standard, it is done by the person responsible for standards and checked and approved by the head of the laboratory. The record on changing necessary data including the date and the signature of the head of the laboratory is a part of the report on the calibration data analysis.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>47</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

#### 10.7.4 Intermediate checks

Intermediate checks of reference standards, which are calibrated outside the laboratory, are not possible (no appropriate equipment is available). Such equipment can only be checked by means of interlaboratory comparisons. The person performing calibrations with this equipment shall check the results (if this is possible based on the results from the past) and the head of the laboratory shall be contacted in the case of suspicion in the correctness of the calibrated value(s). The head of the laboratory decides whether an extra (intermediate) calibration is necessary.

Intermediate checks of the equipment, which is calibrated in the laboratory, are only performed in cases of suspicion in the correctness of operation and in cases when greatest amounts of calibrations are performed with such equipment. Intermediate checks are performed according to the calibration procedures, but instead of a calibration certificate and hand written check report is made. Regular intermediate checks for the equipment in the laboratory are not necessary (this statement is based on the equipment history and on properly defined calibration intervals). The results of intermediate checks shall be stored in the equipment files (»Z:\4-Sistem kakovosti\Zapisi\ OPREMA\Evidenca in status opreme«) by the performer(s) of the checks.

### 10.8 Computer system

#### 10.8.1 Documentation of the computer system

##### 10.8.1.1 Computer system

The computer system consists of PC computers linked in a network.

The **users** in the network have equal priority and enable:

- data input,
- data manipulation.

The documentation of the computer system is divided into:

- hardware documentation (E 02)
- software documentation (E 03 + original software documentation - commercial)

##### 10.8.1.2 Hardware documentation

**Hardware documentation** contents:

- all PCs of the computer system,
- network cards,
- printers and plotters,

##### 10.8.1.3 Software documentation

**Software documentation** contents operating instructions for:

- operation system,
- network,
- word processor,
- data base for control system,
- data base for calibration.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>48</b> of <b>79</b>
	<b>Equipment</b>	Issue No. <b>E-30</b>

## **10.9 Defective equipment**

### **10.9.1 Instruction for removing defective equipment from use**


If it is detected, that equipment:

- does not work,
- does not work properly or there is a doubt about improper functioning,
- gives uncertain results,
- has not been properly used (overloaded, damaged),
- has not been properly maintained or repaired in time,
- has not been calibrated in time

the following actions should be taken:

- portable equipment should be removed from working place and put in the place designated for defective equipment,
- fixed equipment should be equipped with a warning text »NOT FOR USE« - DEFECTIVE EQUIPMENT.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>49</b> of <b>79</b>
	<b>Supplies and services</b>	Issue No. <b>E-30</b>

## 11 SUPPLIES AND SERVICES

### 11.1 Purchasing and contract service policy

Suppliers of new equipment (measuring equipment, computers, furniture, ...) and subcontractors (repairs, cleaning, painting, ...) are chosen in accordance with the following criteria:

- ability to fulfill exactly defined requirements,
- ability to deliver a product or to finish a service in the defined time period,
- quality and fast service,
- price.

A priority is given to the suppliers or subcontractors, with which we have had good experiences in the past, and to those with good reputation (especially suppliers of measuring equipment and standards).

Evaluation of suppliers and subcontractors is based on offers. The laboratory manager is authorized and responsible for choosing the best offers.

After we have got all the offers, we build a list of possible suppliers or subcontractors, which contains:


- type of the product or service,
- names and addresses of checked suppliers res. subcontractors,
- names of contact persons.

In the case of purchasing measuring equipment, we require a calibration certificate of an accredited laboratory. Other equipment (computers, furniture, ...) is inspected by the laboratory staff before installation (100 % inspection). If a purchased product does not meet the requirements, it is returned to the supplier and new equipment is required. If the supplier is not able to deliver suitable equipment, he is deleted from the list of suppliers. Very important criterion for evaluation of suppliers and performers of services is the period of warranty.

### 11.2 Suppliers

#### 11.2.1 Procedure for the assessment of suppliers

- Potential suppliers are selected from catalogues of domestic and foreign professional fairs, from advertisements in professional papers and magazines, by visits of professional stores, from web pages, Accreditation bodies' information, Euromet database, etc.
- The following three methods are used for the assessment of suppliers:
  - reputation of the supplier and experiences with the supplier in the past,
  - technical check of the suppliers' products/services at professional fairs,
  - inspection and tests of purchased products/services.
- The assessment is performed by:
  - the laboratory manager,
  - the quality manager,
  - the personnel performing calibrations.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>50</b> of <b>79</b>
	<b>Supplies and services</b>	Issue No. <b>E-30</b>

- The assessment procedure:
  - suppliers that are able to supply certain product(s)/service(s) with required characteristics are selected,
  - official offers are required from the selected suppliers,
  - potential suppliers are chosen among the selected suppliers on the base of their reputation and our experiences in the past,
  - the chosen suppliers are classified by the product/service price(s) and recorded in the list of approved suppliers.
- The described procedure should be carried out before each purchase and the existing list of approved suppliers should be considered.
- The list of approved suppliers is filed in the folder »4-Sistem kakovosti\Zapisi\OPREMA«. It should contain the following data:
  - the type of the product/service,
  - names and addresses of the approved suppliers,

#### *11.2.1.1 Special procedure for evaluating performers of external calibrations*

The performers of external calibrations can be exclusively European national institutes and the laboratories accredited by an accreditation body, which is a signatory of multilateral recognition agreement.

The quality of the external calibration performers is based on the records of calibration analysis (Ch. 10.7.3), which are stored in the folder »4-Sistem kakovosti/Zapisi/Oprema/Poročila o analizi kalibracij«. The evaluation is performed by using Excel document »Evaluation of the external calibration performers«, which is stored in the same folder as the calibration analysis.


The most important criteria for the evaluation are the following:

- best calibration capabilities (CMC),
- price,
- terms of performance,
- proper communication.
- transportation possibilities,
- results of performed calibration analyses.

## **11.3 Documentation**

### **11.3.1 Procedure for drafting, checking and approval of purchasing documents**

- The quality manager deputy prepares an order, which contains the following information:
  - product/service specifications (name, number of pieces, required tolerances, measuring uncertainty, traceability, service contents, etc.),
  - referring offer,
  - date of delivery specified in the offer,
  - price specified in the offer,
  - exact address of the laboratory and the name of the responsible person.


 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>51</b> of <b>79</b>
	<b>Supplies and services</b>	Issue No. <b>E-30</b>

- The laboratory manager checks and approves the documentation. After that he prepares and sends an application to the executive committee of the Faculty of mechanical engineering. The committee checks the financial state of the laboratory and approves res. rejects the purchase.
- After the purchase has been approved, the laboratory manager sends the order to the supplier. The copy of the order is filed at the accounting department of the Faculty.

## **11.4 Receipt and inspection**

### **11.4.1 Procedure for the receipt and inspection of purchased products**

- The laboratory manager, the quality manager and the staff performing calibrations are authorized and responsible for the receipt of the ordered product(s).
- The staff performing calibrations is authorized and responsible for inspection and testing of purchased product(s).
- If the product is imported, the legal activities (duty etc.) are carried out by the authorized person at the Faculty of mechanical engineering.
- When the product arrives to the Faculty of mechanical engineering, one of the responsible staff members (or the person, quoted on the package) is informed by the faculty post office (the procedure is laid down in the job descriptions of the faculty).
- After the receipt an authorized person unpacks the product. The assembly and installation (if required) are carried out by one or more authorized staff members.
- After the installation the product is inspected (tested) by an authorized person according to the instructions in next chapter. A 100% inspection of product and its components is required.
- If the product meets all the requirements specified in the order, it is accepted and the documentation is signed. In the case of detected defects the supplier is informed immediately.
- In a discussion with the supplier it is stated whether the product is defected or a mistake has been made during the inspection (test). In that case the inspection (test) should be repeated.
- In the case of a defect the product is returned to the supplier or a suitable service is required.
- After the inspection (test) a report should be written by the person performing the inspection (test) and checked by the quality manager. The report is filed in the folder »4-Sistem kakovosti\Zapisi\OPREMA\Poročila o pregledu kupljenih proizvodov in zunanjih storitvah«.
- The use of new equipment must be approved by the laboratory manager (signature on the evidence sheet).

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>52</b> of <b>79</b>
	<b>Supplies and services</b>	Issue No. <b>E-30</b>


#### **11.4.2 Inspection instructions for incoming products**

- The purchased product should first be unpacked and placed in the working position.
- It should be checked if the package is complete in accordance with the specification of components included in the package.
- The specifications of the product should be checked by using the documentation (e.g. measuring range, measuring uncertainty, calibration certificates, proof of traceability, ...)
- The instructions for installation, assembly (if necessary) and use should be collected.
- The product should be assembled. Possible visible damages should be detected during the assembly. If the product is assembled by the manufacturer, one of the authorized staff members should supervise the assembly.
- The product should be installed (if necessary) and the correctness of operation according to the working instructions should be established.
- In the case of measuring or calibration equipment, a calibration with reference standards of measurement should be performed.

### **11.5 Service check**

#### **11.5.1 Procedure and instructions for checking services**


- The following staff members are authorized and responsible for checking services:
  - the laboratory manager,
  - the quality manager,
  - the quality manager deputy.
- After the service has been completed it is checked in a qualitative (e.g. cleaning, replacement of windows, electrical installations, computer service...) or in a quantitative (e.g. service of measuring and calibration equipment, service of the air conditioner,...) way;
  - in the case of a qualitative check the suitability of the service is checked according to the requirements specified in the contract,
  - in the case of a quantitative check a set of measurements is performed (measurements using standards of measurement, temperature measurements, humidity measurements,...) and the quality of the service is evaluated by using the measuring results.
- If the service is evaluated as improper or incomplete, the performer is informed and some corrective actions are required.
- After the service check a report must be written and filed in the folder »4-Sistem kakovosti\Zapisi\OPREMA\Poročila o pregledu kupljenih proizvodov in zunanjih storitvah«. If a service of measuring equipment is checked, the report should be also filed in the folder »4-Sistem kakovosti\Zapisi\OPREMA\Poročila o pregledu kupljenih proizvodov in zunanjih«.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>53</b> of <b>79</b>
	<b>Supplies and services</b>	Issue No. <b>E-30</b>

## **11.6 Storage**

### **11.6.1 Procedures for receipt, storage and issue of products, for stock control and for checking products on stock**

Only consumer goods (paper, cleaning fluids, etc.) are on stock in the laboratory. Therefore, no special procedures are required for receipt, storage, issue and stock control.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>54</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

## 12 PERFORMANCE OF THE WORK

### 12.1 Review of requests, tenders and contracts

The procedure for performing service (calibration and measurement) is the following:


- the client's request which can be in written or in verbal form can be accepted by the permanent performers of calibrations, by the quality manager or by the laboratory manager;
- the request is responded by performers of calibrations, the quality manager or his deputy with a written offer contenting quality description of the service, term of performance and the price; in special cases can the offer be given in verbal form (on client's request, usually for a smaller extent of work). In the case of complex inquiries, staff should consult with the Head of the laboratory. The offer is based on the valid price list approved by the laboratory manager. Before the offer is written, it is checked whether proper equipment, methods, personnel, instructions and standards or client's specifications are available. The capacities shall be checked, too;
- the client sends us an official order, in which he:
  - exactly specifies the contents and the extent of the work,
  - specifies the time period for the performance of the work or accepts our suggestion regarding the time period,
  - confirms an agreement with our offer,
  - specifies special requirements and standards (if necessary),
  - if customer's requirements cannot be fulfilled by using standard methods or written standards, because they are inappropriate or out-of-date, he has to be informed.
- the order is filled in accordance with the procedure in Ch. 12.2; the order (original) stays in the LTM until sending it to the accounting department of the faculty together with the invoice, where is being archived.
- in the case of insufficient capacities, a subcontractor is involved in accordance with the policy in Ch. 14.1;
- the work is performed in accordance with the procedure in Ch. 15 and the invoice is sent to the client;
- if deviations from the agreed procedure appear during the performance of work, the client shall be informed and shall agree (written or verbal agreement) with the changes. Deviation(s) shall be recorded and records shall be stored among the order records.

If a calibration is ordered, we should be aware that we are accredited for the specific type of calibration. When we perform calibrations we are not accredited for, we should issue no certificate with the logotype of the accreditation services.

If ordered work has already been performed in the past, we should use the same working methods. If certain work is accepted for the first time, we should precisely check our capacities and abilities.

The following persons are authorized and responsible for the acceptance of new work:

- laboratory manager,
- quality manager,
- quality manager deputy.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>55</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

Contracted services are performed on the faculty level in research and education fields, **from 2022 also in the field of accredited activity.**

The contract for accredited services that we conclude with our clients must contain the following information:

- Identification of the client: Indication of laboratory data (name, address, contact details) and client data (name, address, contact details).
- Subject of the contract: Clear definition of the accredited services that the laboratory will provide to the client (detailed description of the services, possible limitations, special requirements, etc.).
- Price list and payment terms: Determination of service prices, payment method (e.g., monthly, annually) and payment terms.
- Timeframe: Determination of the timeframe for the providing of the services (date for the start and end of services) and the term of the contract.
- Responsibility and limits: Clearly define the laboratory's responsibility for the quality of services, possible errors or delays.
- Confidentiality and data protection: The contract must contain statements about confidentiality and data protection.
- Contract termination: Definition of the terms of the contract, including the possibility of termination by either party and possible sanctions for breach of contractual obligations.
- General: Include general terms such as conflict resolution and possible annex to the contract.

The quality management representative prepares a draft contract according to the requirements and needs of the client. When the draft contract is ready, it is submitted to the client or his quality representative for review. The client then checks whether the draft contract meets their requirements and whether all the necessary data is included. Once the draft contract has been reviewed and approved by all parties, the contract is prepared for signature.

## 12.2 Performing the work

The following procedure is used for planning the work:

- After the acceptance of the measure, the employee in LTM enters the data in the laboratory diary that is kept on the server in folder »2-Laboratorijski dnevnik«.
- We should check whether we are authorized and qualified to perform the work.
- Each order should be analyzed in order to find out:
  - if all requirements regarding the work are clear,
  - if necessary standards, guidelines and work instructions are available,
  - if the client agrees with using non-standard procedures in the case of absence of standard procedures.
- Necessary work should be specified in detail before beginning of work.
- We should check the availability of sufficient, suitable equipment.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>56</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

- The work should be assigned to the best qualified person(s). If more persons should be involved, we should appoint a team leader. The decision about subcontracting work is taken in accordance with the Ch. 14.
- Every calibration is filled using the program »Kalibracija«. Instructions for filling data is in folder »2-Laboratorijski dnevnik«.
- After the calibration first page of the calibration certificate is created by option »Kalibracija meril« and saved as pdf (filename and location are defined in Ch. 5).
- Following pages of the certificate are created from calibration results (as defined in corresponding SOP) and afterwards transformed to pdf, merged to the file with first page and saved.
- If a certificate contains results of accredited and non-accreditation activities, the difference between these two types of results shall be clearly distinguished. Accreditation mark (SA mark) can be used on such certificates only in case when at least 50 % results are accredited. The mark shall be used together with a note about non-accredited activities. Results marked with # refer to non-accredited activity.
- Normally, no conformity statements and recommendations are written in calibration certificates. If a client explicitly requires such statement or recommendation, his written request shall be filed following the instructions for external correspondence (15.1). When stating conformity, measurement uncertainty shall be considered.
- In case, when giving opinions and interpretation related to the compliance of the measuring instrument with a standard, the identified deviation including measurement uncertainty must be within the boundaries of acceptance set by the standard. The head of the laboratory is authorized and responsible for giving opinions and interpretations. He formulates opinions and interpretations based on the calibration results together with the person authorized for performing relevant activities. All the documents have to be archived appropriately.
- If calibrated instrument should be adjusted (it is showing wrong value in the zero/reference point), the adjustment value (correction) shall be written in the calibration certificate under section »Status of instrument before calibration« (e. g. »The instrument had to be adjusted before calibration. Bias in zero point before calibration:  $O = -2 \mu\text{m}$ «).
- Certificate is digitally signed by the performer of calibration and put in the folder »1-Dokumenti v podpisu«. The laboratory manager, who is regularly checking this folder, approves the certificate with electronic signature and moves it into the folder of the corresponding performer of calibration. The performer of calibration shall move the file (certificate) into the folder where raw version was created. By doing this, a certificate in electronic form is completed.
- All records of calibration are treated as defined in Ch. 6.2.


### **12.3 Policy regarding design and development activities**

New methods or procedures are developed when no standard procedures res. methods are available and when a client is not able to provide us with his own or already used methods and procedures.

A new measuring procedure (method) must assure a correct result of a calibration.

We should get an agreement from the client before using a new non-standard procedure or method. If the client has any objections, the new procedure should not be used.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>57</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

New methods and procedures are designed and developed by the staff performing calibrations and by the staff developing new measuring methods and devices. A new procedure or method should be approved by the laboratory manager or by the quality manager before use.

## 12.4 Calibration procedures

The list of the available calibration procedures is in the folder Spiski (see Ch. [5.1](#)).

## 12.5 Validation of the software used for calibration

Entire software used for calibration must be validated using the following procedure:

- values calculated by the software are compared with the manually calculated values. Manual calculation is based on the values given by the measuring device (e.g. read from the display) for the smallest, middle and the greatest measuring value.
- the calibration procedure must be followed precisely when calculating manual values,
- proper validation method is created for every calibration procedure,
- procedure, calculations and the results of the validation for every calibration procedure are archived,
- the revision numbers of validated software must be kept in the records.

## 12.6 Quality control of performed work

Quality manager and his deputy are responsible for the quality control of the performed work.


The control is performed in the following way:

- results in calibration certificates are checked,
- performance of work is checked during internal audits,
- client's responds are checked (complaints and remarks),
- best measurement capabilities of calibration procedures are regularly checked by:
  - intercomparisons on national and international level,
  - research in the field of equipment, procedures and environmental influences,
- accredited calibration procedures are checked by expert assessors of accreditation bodies (evaluation of measuring uncertainty, suitability of the procedures, performance of calibrations, calibration certificates, environmental conditions).

### 12.6.1 Intercomparisons

Intercomparisons are the most important parameter of detecting quality of performed measurements and calibrations. Therefore the laboratory is participating at all intercomparisons organized by national accreditation body, European accreditation or EURAMET. The aim of the laboratory is also to take part in other bilateral or multilateral intercomparison schemes in the limits of its financial possibilities and to organize and conduct such intercomparisons in the frame of research projects.

Head of the LTM writes a plan of intercomparisons. In 4-years period LTM will participate in at least one intercomparison in every subgroup from the accreditation scope (4.1.x and 4.2). The plan is stored in the folder »4-Sistem kakovosti\Zapisi\Interkomparacije«.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>58</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

Acceptance of our results in intercomparisons is determined by following acceptance criteria:

- for Euramet intercomparison, criteria for acceptance of results are set by the pilot laboratory;
- for other intercomparisons,  $E_n$  is calculated, the result is acceptable when  $E_n < 1$ .

After the analysis of intercomparison results report is written and saved in the folder for quality system records.

## **12.7 Work instructions**

### **12.7.1 List of available work instructions**

A list of available work instructions is in the folder Spiski (see Ch. 5.1).

### **12.7.2 Documentation**

Work instructions are stored in the folder »Work instructions«, which is located in the calibration room (room D1 004 - Microclimatic chamber) and in folder »4-Sistem kakovosti/Delovna navodila«.

## **12.8 Security**

### **12.8.1 Protection against unauthorized entering the measuring rooms**

The procedure is specified in the Ch. 9.

### **12.8.2 Instructions on how to act in the case of emergency**


In the case of natural accidents and fire the following instructions should be taken into consideration:

- A fire extinguisher HL-3 for extinguishing all kinds of fire (types B, C and E) should be used in the case of fire breaking out (e.g. caused by electricity or inflammable fluids). One extinguisher is located in each laboratory room. The extinguishers should be checked periodically - each year (the maintenance service of the Faculty is responsible for periodic checks).
- The person detecting fire or other accident should immediately inform the Faculty management and the maintenance service (phone numbers are in the internal phonebook). After that he (she) should try to help in the accident.
- If fire is too strong and/or if people are hurt, we should immediately call a fire brigade (phone No. 112) and/or rescue service (phone No. 112).
- In the case of lightning hit and/or power failure, which can lead to breakdown or failure of devices measuring over a long period of time (especially when nobody is present in the laboratory), we use UPS (uninterruptable power supply).
- Falls or slips, which were caused by wet or slippery floor, laid electric cables and other reasons, are prevented by keeping working surfaces tidy / obstacle free, with immediate action in the case of fluid spills (wiping), as well as sufficient care and attention at work.

### **12.8.3 Instructions for the use of personal safety equipment**

#### *12.8.3.1 Protecting clothes*

In air-conditioned rooms we should wear clothes, suitable for laboratory and not for the outside conditions.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>59</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

The following protecting means enable safety use of the equipment:

- protecting coats (white colour),
- protecting cotton gloves (white colour),
- protecting plastic gloves.

#### *12.8.3.2 Additional safety measures*

The following safety guidelines should be concerned when working with the equipment:

- Proper lifts and transportation means should be used for transportation in order to enable safe and effective work.
- Illumination of measuring rooms should fulfil the requirements in the chapter 9 - Facilities.
- After the work all tools, instruments and auxiliaries used should be cleaned (oiled, if necessary) and put into their places.
- A device LAMBRECHT, type TH-252 with monthly print -out for continuing registration of important physical values (temperature, air pressure, humidity) is placed in the measuring room.

## **12.9 Objects of calibration**

### **12.9.1 Procedures for receipt, storage and issue of calibration objects**

Objects of calibration should be checked at the time of receipt:

- identification numbers on items must be the same as those on the order,
- number of items must be the same as the specified number on the order,
- all detected damages must be registered using the form »Obr 04-Zapis o neustreznosti merila.doc« in the folder »Obrazci« (see Ch. 5.1).
- the documentation must be complete.

In the case of a doubt about the suitability of the calibration object/sample or if the object/sample doesn't comply with the enclosed description, we must consult the client before continuing and record or properly document the results of this consultation. If the client requires the calibration of the object/sample anyway and recognizes its deviation from the specified conditions, the certificate must indicate, which results might have been affected by the deviation. In addition, we provide customer's information about the influences on the validity of results in the certificate.

Reception of the objects is recorded using a software program »Kalibracija«, using an option »Sprejem meril« (reception of the measure). Instructions for using the software are in the folder »Računalniška programska oprema – E 03«.

Thereby generated record »Prevzem merilnega orodja« is saved in electronic form, as defined in Ch. 5.1.

### **12.9.2 Identification system for calibration objects**

Each calibration/test object is recorded into the Excel document »2-Laboratorijski dnevnik« and stored in the packaging until the start of the calibration.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>60</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

### 12.9.3 Handling of calibration objects

The following instructions regarding handling of items should be followed:

- Objects of calibration should be handled in such a way, that their characteristics are not changed during the calibration. The changes of characteristics can be caused by mechanical damages, overloading, corrosion, contamination etc.
- If objects are damaged, lost etc. during the calibration, the client should be informed immediately and a protocol about damage should be written.

The following instructions regarding disposal of objects of calibration should be followed:

- Objects should be properly packed and protected in the case of sending by mail.
- Proper transportation means should be chosen.
- All mails and personal receipts of calibrated objects should be registered.


### 12.9.4 Procedures for storing objects of calibration

- After the receipt and identification objects of calibration should be cleaned and put on a special place designated for objects that are not yet calibrated (in the room D1 005).
- If the calibration is not performed on the day it was received, objects should be properly protected against the environment influences. If the objects have been in an original package, we do not unpack them. If the objects have not been properly packed, we should oil them with special oil and put into cardboard boxes.
- We should handle the objects with special care during packing and classifying in order to avoid mechanical damages. Objects should be packed separately.
- A calibration procedure can be started after the temperature of the object has reached the reference value (20 °C). No chemical methods (fluid nitrogen bath, etc.) are allowed for cooling objects of calibration and no intensive heating is allowed for warming up objects of calibration. Intensive cooling and heating can cause permanent deformations.
- Work instructions should be followed precisely during calibration.
- We should take care that the work conditions are within the prescribed limits.
- After calibration, objects should be oiled again (if appropriate) and packed in order to avoid mechanical damages.
- Calibrated items are put on the designated place (in the room D 005).
- Objects of calibration can be handled only by authorized staff members (laboratory manager, quality manager, staff performing calibrations). Other persons are not allowed to touch the objects.

### 12.9.5 Procedures for delivering objects of calibration

At handing over/delivery following rules apply:

- when delivering by mail objects have to be properly packed in order to avoid mechanical damages,
- when delivering by mail both the letter (form) »Obr 13-Spremni dopis za pošiljanje meril.doc«, stored in the folder Obrazci (see Ch. 5.1), and the list of the objects (Prevzem merilnega orodja) are to be included. If not all objects from the list are send, all redundant are to be strike through.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>61</b> of <b>79</b>
	<b>Performance of the work</b>	Issue No. <b>E-30</b>

- when objects are handed over to the client, he/she confirms a completeness of the list of the objects with a signature on the list. The signed list is kept for the time of complaint, as stated on the list.
- all mail delivery must be registered.

## **12.10 Software for calibration**

### **12.10.1 Procedure for maintaining and up-dating software for calibrations**

- software for calibrations can be:
  - bought with a measuring device,
  - made in the laboratory;
- the list of software is kept in the folder »Computer software – E 03«;
- instruction for use of software are kept in the folder »Computer software – E 03«;
- all software used for calibrations shall be validated before first use in accordance with the policy in Ch. 12.5. Records of validations are kept in the folder »Validacija programske opreme za kalibracije«;
- original of a valid software version (floppy disc, CD or other medium) is stored in the microclimatic chamber in D1 004, except for the CMM, which is kept near the device;
- the user uses a copy of original software;
- quality manager is responsible for managing lists of software;
- software is up-dated (a new version of commercial software is purchased or self-developed software is changed) in a case, when a user detects that the old version is not suitable any more (because equipment is renewed or calibration demands change);
- the head of the laboratory decides to change or up-date of software after an initiation of user or after a distributor has informed us about issuing a new version.

### **12.10.2 Procedure for filing changed (old) versions of calibration software**

- an obsolete version of software, which was replaced with a new one, is filed in the archive of documentation (case F in the room D1 004);
- software carrier (floppy disc, CD, ...) shall be marked with a yellow label »Invalid version«;
- the obsolete version shall be stored for five years after the last use;
- quality manager is responsible for filing obsolete version.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>62</b> of <b>79</b>
	<b>Calibration on site</b>	Issue No. <b>E-30</b>

## 13 CALIBRATION ON SITE

### 13.1 Quality policy

Quality policy for all calibrations on site is equal to the policy for in the laboratory. Appropriate procedures must be established for all calibrations on site. These procedures should include all specific instructions for calibration on site. Measuring uncertainty should be evaluated concerning conditions of calibration on site. Therefore, special attention is paid to measurement and records of calibration conditions. Responsible and authorized personnel for calibration on site are the same as for calibration in the laboratory. The personnel must be precisely informed about the regulations stated in this document. No hired personnel or subcontractors are involved in calibration on site. Quality manager includes the review of calibration on site in regular audits of the quality system. Client who orders calibration on site has the same rights and possibilities (e.g. possibility of complaint, presence at calibration) as the one who orders calibration in our laboratory.

The laboratory manager is personally responsible for the insurance of the personnel and the equipment during the period of transport and calibration on site.

Quality policy was defined by the laboratory manager and approved by the dean of the Faculty of Mechanical Engineering. Signed original is in Z 09.

### 13.2 Organization

#### 13.2.1 Organization scheme

There is no special scheme for calibration on site. Calibrations are performed by the personnel from the department »Measurement and calibrations«.

#### 13.2.2 Personnel

The personnel involved in calibration on site have the same authority, duties and responsibility as for calibration in the laboratory. Requirements for the personnel performing calibration on site are the same as for personnel performing calibrations in the laboratory.

#### 13.2.3 Equipment

For calibrations on site we use the same equipment (also standards) as for calibrations in the laboratory. The equipment should always be transported in proper packages for the protection against damages. No special requirements for transportation means or conditions are necessary. Equipment used for calibration on site is marked in the equipment list in **the document »Plan kalibracij«**.

When measuring equipment is used outside the laboratory, it shall be recorded in the Excel document »Iznos merilne opreme iz laboratorija.xls«. The document is stored in the folder »Laboratorijski dnevnik«. Each entry shall contain exit dates and condition of the measuring equipment after the return.

#### 13.2.4 Procedures

SOP's including specific instructions for calibration on site are used. General procedures and instructions for planning, performing and activities after calibration on site are defined in chapters 13.3, 13.4 and 13.5.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>63</b> of <b>79</b>
	<b>Calibration on site</b>	Issue No. <b>E-30</b>

### 13.3 Planning of calibration

- When an official order is received, the client is asked for the following data:
  - data about the equipment to be calibrated and the drawings of the equipment if necessary for making special fixtures etc.,
  - the most appropriate term of calibration according to the stability of the conditions in the room, where calibration will be performed,
  - possibilities for accessing place of calibration (access by car and transport of equipment),
  - if device to be calibrated/inspected requires specially educated operator (e.g. coordinate measuring machines with different software), the client should make an operator available for the time of calibration.
- If necessary, it is agreed with the client about the machining of special fixtures (at his or at our place) and about additional expenses for these fixtures.
- Term of calibration is planned and agreed with the client.
- Person, who received an order (authorized and responsible persons for receiving orders are the same as for calibrations in the laboratory), informs the head of the laboratory about the planned calibration.
- The head of the laboratory (or the deputy in his absence) defines the person (s) who will perform the calibration and approves all necessary costs (travel costs, insurance, additional costs for performing work, hotel, etc.).
- Before the calibration the client is required to send written and approved order stating the equipment to be calibrated.
- Person who will perform the calibration must enter the list of necessary equipment that will be taken out of the laboratory in the Excel document »Iznos merilne opreme iz laboratorija.xls«, which is stored in folder »Laboratorijski dnevnik«.
- Before leaving the laboratory the equipment should be checked and protected against possible damages by the person who will perform the calibration. The head of the laboratory arranges proper insurance for the equipment.

### 13.4 Performance of calibration

- Performer(s) of calibration must bring an official document (travel order) and his identification document with him.
- Performer(s) should know the contact person of the client who will arrange documents for bringing the equipment in and out of client's premises.
- Before performing calibration the performer should check the equipment to be calibrated and auxiliary equipment together with the responsible person of the client in order to detect existing defects, damages or malfunction.
- The performer fills the form »Obr 07-Zapisnik o stanju merilne opreme pri kalibr. na terenu.doc« about the condition of the equipment.
- The equipment that is not in proper condition is not calibrated.
- The performer of calibration checks the room and writes the conditions into the calibration record. During the calibration temperature and other important conditions should be measured



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>64</b> of <b>79</b>
	<b>Calibration on site</b>	Issue No. <b>E-30</b>

and recorded (at least before and after the calibration). Therefore, calibrated sensors should be brought on site (if it is calibrated with laser interferometer, included sensors are used, in other cases temperature is measured using system TEMP 14).

- Calibration is performed in accordance with the calibration procedure, which should be available to the performer on site.
- Before the calibration the equipment (instruments, standards) used for calibration should be thermally stabilized. The time and the manner of stabilization depend on the equipment used and are described in calibration procedures that describe calibration on site.
- If special operator (client's personnel) should operate the calibrated device, detailed information about measurement strategy (measuring points - positions, measurement force, number of repeated measurements in measurement positions, contents of measurement protocol, ...) should be provided to him by the performer of calibration.
- During the calibration the conditions should be observed on their stability and deviations. The performer should tell the personnel of the client not to open doors or windows unless it is really necessary and the number of persons in the room should be as low as possible. The attention should be paid to the transportation means (if calibration is performed in production room) which should be avoided in the surrounding of calibrated device.
- Calibration record should be written during calibration using appropriate forms.
- After the calibration equipment should be packed and the number of pieces should be checked according to the list of equipment.
- The condition of calibrated equipment is checked again together with the authorized person of the client and the record is signed by both persons.
- Calibration certificate is not written on site. It is written after the calibration in the laboratory following common procedure for writing calibration certificates.

### **13.5 Activities after calibration**

- After a calibration the equipment should immediately be returned to the laboratory even if the performer returns very late (in no case it should be carried home or let in a car).
- The performer of calibration is personally responsible for the equipment that was not returned immediately.
- When the equipment is returned to the laboratory, the performer should check completeness according to the list. After that the equipment should be properly protected (oiled, packed etc.) and placed back to its usual place. Date of return and the status of the measuring equipment must be entered in Excel document »Iznos merilne opreme iz laboratorija.xls«.
- Calibration after returning is not foreseen (because of the nature of the equipment used on site it is not necessary). However, it can be suggested by the performer of the calibration if he thinks it is necessary because of special reasons (it was drooped or hit, ...).
- The performer of the calibration completes the order (all necessary documents are written and objects of calibration are recorded in accordance with the ordinary rule for calibration in the laboratory) and writes a calibration certificate, which is then sent to the client. In the calibration certificate has to be stated, that the calibration was carried out on site, location has to be stated.



 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>65</b> of <b>79</b>
	<b>Calibration on site</b>	Issue No. <b>E-30</b>

## **13.6 Audit and review**

### **13.6.1 Audit of performance of calibration on site**

Quality of calibrations on site is audited once a year by the head of the laboratory. The audit is not included in the annual plan, but the most convenient calibration is chosen regarding to received orders. The report on external audit is included in the annual internal audit report. The report written using the form »Obr 09-Poročilo o interni presoji.doc« in the folder Obrazci (see Ch. 5.1). Report is saved as \*.pdf and digitally signed.

### **13.6.2 Management review**

Calibrations on site are treated by management review in the same way as the calibrations performed in the laboratory. We should evaluate conformity of the performance with written procedures and policy, and adequacy of the procedures in respect with experiences and remarks of the performers of calibrations.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>66</b> of <b>79</b>
	<b>Subcontracting</b>	Issue No. <b>E-30</b>

## **14 SUBCONTRACTING**

### **14.1 Policy regarding subcontracting**

Calibrations are subcontracted only in a case of equipment defect that cannot be repaired in a proper time period (calibration schedule cannot be followed).

Subcontractors must be accredited.

Calibrations can be subcontracted only in agreement with clients (written and signed agreement).

Only the original report (certificate) issued by the subcontractor is allowed to be given to the client. The results of the subcontractor are not allowed to be used for issuing our own certificate(s).

### **14.2 Procedure for subcontracting calibrations**

- The laboratory manager decides whether subcontracting calibration is necessary and chooses a subcontractor. Only accredited subcontractors can be chosen.
- The laboratory manager calls the subcontractor and makes sure that the subcontractor has sufficient free capacities available and that he is capable of performing the calibrations in the defined time.
- The quality manager gets the client's written agreement with subcontracted calibrations.
- The laboratory manager prepares a contract in which he exactly defines the price of the calibration, the time for completing the calibration, required measuring uncertainty and the contents of the calibration report. The contract is checked by the legal service of the Faculty of mechanical engineering.
- The objects of calibration should be properly marked and sent to the subcontractor together with necessary documentation.
- After the calibration has been completed, we go to the subcontractor to get the objects, the calibration reports, and the documentation (we never use mail service to get these items).
- The client gets the original report/certificate issued by the subcontractor.
- The calibration reports written by subcontractors should be filed (Z 06). The subcontractor is required to give us entire documentation of the calibration (including calculation, notes etc.).
- The following procedure is the same as by usual calibrations.

### **14.3 List of accredited subcontractors**

The list of accredited subcontractors is in Z 06.

### **14.4 List of subcontracted calibrations**

The register of subcontracted calibrations is in Z 06.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>67</b> of <b>79</b>
	<b>Cooperation with clients</b>	Issue No. <b>E-30</b>

## 15 COOPERATION WITH CLIENTS

### 15.1 Visits in the laboratory and communication with clients

- The client should get the opportunity to:
  - enter the laboratory and control the calibrations,
  - get the data about the conditions, methods and results (including calculations) of the calibrations performed for them,
  - communicate with the staff performing calibrations and with the responsible staff (explanations etc.).
  - access to the operating conditions (LTM web page).
- Electronic correspondence with clients is saved in its original format right after receiving or sending an e-mail. Received and sent e-mails are stored in Outlook in the laboratory e-mail account [ltm@um.si](mailto:ltm@um.si). Only correspondence, which influences quality of performed calibration (offers, explanations, complaints...) are stored, all unimportant mails are deleted promptly. Correspondence is archived for 2 years.
- Clients can get copies only upon written request. Copies are sent by registered mail to get client's receipt.
- The laboratory manager, the quality manager, and the staff performing calibrations are authorized and responsible for the communications with clients.
- The staff should introduce itself before each communication with a client.
- The client should get the name of the person to whom he (she) can mail the post or send a fax (orders, documentation, requirements, complaints, etc.).
- Clients should be informed about the changes of the address, phone number, fax number, etc.
- When communicating with clients we should consider their requirements, wishes, and suggestions. However, some limitations regarding our quality policy, work plans etc. should be respected.

### 15.2 Evaluation of client's satisfaction

Questionnaires about satisfaction with the performed service (calibration) are sent to the clients once a year. Survey can be done per post or online. The questionnaires of the client's satisfaction with the completed service (form »Obr 24 or online questionnaire«) are sent or delivered to all subscribers of our services in the past year. Questionnaires are sent together with franked envelope which is addressed to the quality management. Online questionnaires are sent to customer e-mail addresses (customer base).

The quality manager analyses collected answers and presents them at the management review.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>68</b> of <b>79</b>
	<b>Complaints</b>	Issue No. <b>E-30</b>

## 16 COMPLAINTS

### 16.1 Procedure for dealing with complaints


- A person receiving a complaint should note the following data:
  - the name and the address of the client and the name of the contact person,
  - date,
  - service to which the complaint is referring,
  - date of performance of the service,
  - contents of the complaint.
- The noted data are given to the quality manager.
- The quality manager enters a report about the complaint/announcement in the Excel document »Register pritožb« and informs the laboratory manager.
- The laboratory manager should be informed about the complaint on the day it was received. In his absence all necessary actions are taken by the quality manager.
- The laboratory manager sends a written confirmation of receiving the complaint/appeal containing a short description of the complaint to the customer.
- The laboratory manager analyses the complaint in cooperation with the quality manager and the person performing the service, and defines a procedure for handling it. The analysis and the procedure for handling the complaint should be added to the report about the complaint.
- The quality manager calls the client and explains him the decision of the laboratory management regarding the complaint.
- If it is necessary to repeat or complete the service, it is done on our own expenses (including expenses of transport, mail, etc.) in the time period agreed with the client.
- The expenses regarding a complaint should be precisely specified and included into the report about the complaint.
- The report about a complaint is sent to:
  - the client,
  - the laboratory manager,
  - the quality manager,
  - the documentation file of the laboratory (reports about a complaints are stored in the folder »Z:\2-Laboratorijski dnevnik\Register pritožb«).
- If a quality system deficiency is detected during the analysis of a complaint, a corrective action should be taken immediately.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>69</b> of <b>79</b>
	<b>Complaints</b>	Issue No. <b>E-30</b>

## 16.2 Instructions for keeping the register of complaints

The register of complaints (»Z:\2-Laboratorijski dnevnik\Register pritožb«) is maintained by the quality manager. The following information should be included in the register for each complaint:

- name and address of the client,
- date of the complaint,
- service the complaint is referred to,
- date of the service completion,
- all correspondence with client,
- report about the complaint,
- analysis of the complaint,
- decision whether the service should be redone,
- detected quality system deficiency,
- corrective actions.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>70</b> of <b>79</b>
	<b>Cooperation with accreditation bodies</b>	Issue No. <b>E-30</b>

## **17 COOPERATION WITH ACCREDITATION BODIES, CALIBRATION INSTITUTIONS AND AUTHORITIES**

Procedure for cooperation with accreditation bodies applies also for cooperation with authorities in the field of metrology (e.g. MIRS):

- responsible person: laboratory manager,
- contact person: quality manager and laboratory manager,
- documentation sent to the accreditation body:
  - quality manual,
  - calibration procedures (SOP).
- documentation available to the accreditation body during assessment or surveillance visit:
  - entire laboratory documentation, records, etc. without exceptions,
- access to the spaces and equipment:
  - unlimited access, accompanied by at least one member of the permanent laboratory staff,
- availability of information about the laboratory to the accreditation body:
  - laboratory management will send to the accreditation body all the required information necessary for the maintenance of accreditation (questionnaires, telephone information, ...),
- arrangements of assessments and surveillance visits:
  - dates of visits will be agreed concerning the possibilities of the laboratory and the accreditation body.

LTM actively cooperates with other calibration laboratories and inspection bodies concerning intercomparisons (see ch. 12.6.1), with standardization organisations (SIST) and authorities from the field of metrology in the process of preparing metrology standards. Head of the laboratory is responsible for that.

 LABORATORIJ ZA TEHNOLOŠKE MERITVE	<b>QUALITY MANUAL</b>	Page No.: <b>71</b> of <b>79</b>
	<b>Scope of accreditation – ISO 17025:2017</b>	Issue No. <b>E-30</b>


## **18 SCOPE OF ACCREDITATION ACCORDING TO ISO 17025:2017**

Scope of accreditation is on the SA web page:

<http://www.slo-akreditacija.si/accreditation/univerza-v-mariboru-fakulteta-za-strojninstvo-2/>

Valid annex to the LK - 003 Accreditation Certificate is in Annex 1.

## ANNEX I:

 **SLOVENSKA  
AKREDITACIJA**

Reg. št. / Ref. No.: 3150-0003/10-0014  
Velja od / Valid as of: 23. marec 2023  
Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of: 10. maj 2022

Akreditacija je veljavna do preklica. Veljavnost je mogoče preveriti na spletni strani SA, [www.slo-akreditacija.si](http://www.slo-akreditacija.si).  
This accreditation shall remain in force until withdrawn. Information on current status is available at the SA website, [www.slo-akreditacija.si](http://www.slo-akreditacija.si).

**PRILOGA K AKREDITACIJSKI LISTINI**  
**Annex to Accreditation Certificate**

**LK-003**

**1 AKREDITIRANI ORGAN / Accredited body**

UNIVERZA V MARIBORU, FAKULTETA ZA STROJNIŠTVO  
Smetanova ulica 17, 2000 Maribor

**2 ZAHTEVE ZA USPOSOBLJENOST / Competence Requirements**

SIST EN ISO/IEC 17025:2017

**3 OBSEG AKREDITACIJE / Scope of accreditation**

V okviru te akreditacijske listine Slovenska akreditacija priznava akreditiranemu organu usposobljenost za opravljanje naslednjih dejavnosti: / SA hereby recognizes the accredited body as being competent to perform the following activities:

**3.1 Skrajšan opis obsega akreditacije / Brief description of the scope**

Kalibriranje na naslednjih področjih in naštetih pod-področjih / Calibration in the following fields and the specified sub-fields:

- o Dimenzionalne veličine / Dimensional Quantities:
  - Dolžina / Length: končna merila dolžine, črna merila, instrumenti za merjenje dolžine, končna merila premera, koordinatne merilne naprave / End gauges, Line scales, Length instruments, Diameter gauges, Co-ordinate measuring machines;
  - Oblika / Form: merila ravnosti / Flatness gauges;

OB05-32 \* Izdaja / Revision: 8 Stran / Page: 1 / 8



SLOVENSKA  
AKREDITACIJAPriloga k akreditacijski listini  
Annex to Accreditation Certificate

Velja od / Valid as of

Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of

Akreditacija je veljavna do preklica. Veljavnost preveriti na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at

LK-003

23. marec 2023

10. maj 2022

[www.slo-akreditacija.si](http://www.slo-akreditacija.si)

- Navojne veličine / Thread quantities: navojni trni, navojni obroči / thread plugs – plain, thread rings – plain;
- Kot / Angle: merila kota, merilniki nagiba / Angle gauges, Clinometers;
- Lasersko sevanje / Laser radiation: frekvenčno stabilizirani laserji / Frequency stabilized lasers.

PRILOGA K AKREDITACIJSKI LISTINI  
Annex to Accreditation Certificate

LK-003

AKREDITIRANI ORGAN / Accredited body

LABORATORIJ ZA MERITVE IN KONTROLO  
Slovenski inštitut za strojništvo  
Slobovska ulica 17, 1000 Ljubljana

ZAHTEVE ZA USPOSOBLJENOST / Competence Requirements

SLET 23. MAREC 2023

OBSEG AKREDITACIJE / Scope of accreditation

V okviru akreditacije laboratorija (v nadaljevanju akreditirani organ) se določajo naslednje dejavnosti, ki vključujejo merjenje in kontrolo:

Merjenje navojnih veličin (v nadaljevanju merjenje):

Merjenje kota (v nadaljevanju merjenje):

3.1. Opis akreditacije / Brief description of the scope

Kar nekaj akreditirani organ (v nadaljevanju akreditirani organ) opredeljuje v naslednjem seznamu akreditacije in v skladu s tem:

v) Oprema / Equipment

- Laserski kotni merilniki / Laser angle gauges

- Laserski merilniki kota / Laser angle gauges

- Obroč / Thread plug


 SLOVENSKA  
AKREDITACIJA

 Priloga k akreditacijski listini  
Annex to Accreditation Certificate  
Velja od / Valid as of  
Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of  
Akreditacija je veljavna do preklica. Veljavnost preveriti na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at

LK-003

23. marec 2023

10. maj 2022

www.slo-akreditacija.si

### 3.2 Podroben opis obsega akreditacije / Detailed scope of accreditation

#### 3.2.1 Laboratorij za tehnološke meritve, Smetanova ulica 17, 2000 Maribor

Tabela / Table 1 – Kalibracije v laboratoriju / In-lab calibrations

Št. No.	Merjena veličina, (pod)področje, oz. merilni instrumenti in/all območje (merjene veličine). <i>Measured quantity, (sub-)field, and/or instruments, and/or range (of measured quantity).</i>	Območje (merjene veličine) ali Omejitve, pogoji, vplivne veličine.*** <i>Range (of measured quantity) or Limitations, conditions, influence quantity.***</i>	Kalibracijska in merilna zmogljivost (CMC) izražena kot razširjena negotovost.* <i>Calibration and measurement Capability (CMC) Expressed as an Expanded Uncertainty.*</i>	- Tip kalibracijske metode (opcija) - Kalibracijski postopek - Merilni instrumenti (opcija)** - Opombe - Type of calibration method (option), - Internal calibration procedure - Measuring instruments (option)** - Remarks
<b>DIMENZIONALNE VELIČINE / Dimensional Quantities</b>				
<b>Dolžina / Length (L)</b>				
				L – merjena dolžina / measured length
<b>Končna merila dolžine / End gauges</b>				
	Mejna vzporedna dolžinska merila - merilne kladice <i>Gauge blocks</i>			- Interna postopka / Internal procedures SOP 4, SOP 16
1.		(0,5 do/to 100) mm	$\sqrt{(35 \text{ nm})^2 + (0,5 \cdot 10^{-6} \cdot L)^2}$	- Jeklene merilne kladice / Steel gauge blocks SOP 4
2.		(>100 do/to 1000) mm	$\sqrt{(70 \text{ nm})^2 + (0,4 \cdot 10^{-6} \cdot L)^2}$	- Jeklene merilne kladice / Steel gauge blocks SOP 16
3.		(0,5 do/to 100) mm	$\sqrt{(50 \text{ nm})^2 + (0,55 \cdot 10^{-6} \cdot L)^2}$	- Keramične merilne kladice / Ceramic gauge blocks SOP 4
4.		(0,5 do/to 100) mm	$\sqrt{(50 \text{ nm})^2 + (0,9 \cdot 10^{-6} \cdot L)^2}$	- Merilne kladice iz karbidne trdine / Tungsten carbide gauge blocks SOP 4
	Stopničasta merila <i>Step gauges</i>			- Interni postopek / Internal procedure SOP 40
5.		(0 do/to 1500) mm	$\sqrt{(0,1 \mu\text{m})^2 + (0,5 \cdot 10^{-6} \cdot L)^2}$	
	Debelinska merila <i>Thickness gauges</i>			- Interni postopek / Internal procedure SOP 29
6.		(0 do/to 100) mm	$0,3 \mu\text{m} + 1,6 \cdot 10^{-6} \cdot L$	
7.		(100 do/to 1000) mm	$2,1 \mu\text{m} + 3,3 \cdot 10^{-6} \cdot L$	
	Zevna merila <i>Gap gauges</i>			- Interna postopka / Internal procedures SOP 30, SOP 31
8.		(0 do/to 100) mm	$0,6 \mu\text{m} + 0,8 \cdot 10^{-6} \cdot L$	
9.		(100 do/to 1000) mm	$2,1 \mu\text{m} + 3,3 \cdot 10^{-6} \cdot L$	
<b>Črtna merila / Line scales</b>				
	Toga črtna merila <i>Rulers</i>			- Interni postopek / Internal procedure SOP 21
10.		(0 do/to 500) mm	$\sqrt{(90 \text{ nm})^2 + (1,1 \cdot 10^{-6} \cdot L)^2}$	
11.		(0 do/to 3000) mm	$1,8 \mu\text{m} + 2,1 \cdot 10^{-6} \cdot L$	
	Tračna merila <i>Tape measures</i>			- Interni postopek / Internal procedure SOP 23
12.		(0 do/to 200) m	$10 \mu\text{m} + 12,5 \cdot 10^{-6} \cdot L$	
	2D mreže <i>2D grids</i>			- Interni postopek / Internal procedure SOP 38





**SLOVENSKA  
AKREDITACIJA**

Priloga k akreditacijski listini  
Annex to Accreditation Certificate  
Velja od / Valid as of  
Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of  
Akreditacija je veljavna do preklica. Veljavnost preveriti na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at

LK-003

23. marec 2023

10. maj 2022

www.slo-akreditacija.si

Št. No.	Merjena veličina, (pod)področje, oz. merilni instrumenti in/ali območje (merjene veličine). Measured quantity, (sub-)field, and/or instruments, and/or range (of measured quantity).	Območje (merjene veličine) ali Omejitve, pogoji, vplivne veličine.*** Range (of measured quantity) or Limitations, conditions, influence quantity.***	Kalibracijska in merilna zmogljivost (CMC) izražena kot razširjena negotovost.* Calibration and measurement Capability (CMC) Expressed as an Expanded Uncertainty.*	- Tip kalibracijske metode (opcija) - Kalibracijski postopek - Merilni instrumenti (opcija)** - Opombe - Type of calibration method (option), - Internal calibration procedure - Measuring instruments (option)** - Remarks
13.		do/to 300 mm x 200 mm	$\sqrt{(0,32 \mu\text{m})^2 + (4,2 \cdot 10^{-6} \cdot x)^2 + (1,6 \cdot 10^{-6} \cdot y)^2}$ za x – os $\sqrt{(0,32 \mu\text{m})^2 + (10^{-6} \cdot x)^2 + (1,6 \cdot 10^{-6} \cdot y)^2}$ za y – os	
Instrumenti za merjenje dolžine / Length instruments				
	Naprave za kalibracijo mejnih vzporednih dolžinskih meril Gauge block comparators			- Interni postopek / Internal procedure SOP 2
14.		(0 do/to 100) mm	20 nm + 0,2 · 10 <sup>-6</sup> · L	
	Naprave za kalibracijo merilnih uric Dial gauge testers			- Interni postopek / Internal procedure SOP 12
15.		(0 do/to 125) mm	0,1 μm + 2,5 · 10 <sup>-3</sup> · L	
Merilne urice, tipala, instrumenti z uricami / Dial gauges, probes, instruments with dials				
	Merilne urice Dial gauges			- Interni postopek / Internal procedure SOP 8
16.		(0 do/to 50) mm	0,9 μm + 2,5 · 10 <sup>-3</sup> · L	
	Merilniki globine profila pnevmatik Tire tread depth gauge			- Interni postopek / Internal procedure SOP 8
17.		(0 do/to 50) mm	2,5 μm	
	Merilniki z urico – debelinski, zunanji, notranji Instruments with dials – thickness, external, internal			- Interni postopek / Internal procedure SOP 8
18.		(0 do/to 100) mm	0,7 μm + 1,2 · 10 <sup>-3</sup> · L	
	Precizna tipala Precise probes			- Interni postopek / Internal procedure SOP 15
19.		(0 do/to 100) mm	$\sqrt{(30 \text{ nm})^2 + (10^{-3} \cdot L)^2}$	
	Dvotočkova vijačna merila (zunanja in notranja) 2 point micrometers (external and internal)			- Interni postopek / Internal procedure SOP 5
20.		(0 do/to 1000) mm	1 μm + 4 · 10 <sup>-6</sup> · L	
	Tritočkova vijačna merila 3 point micrometers			- Interni postopek / Internal procedure SOP 5
21.		(4 do/to 275) mm	1 μm + 4 · 10 <sup>-6</sup> · L	
	Pomilna merila Vernier callipers			- Interni postopek / Internal procedure SOP 6
22.		(0 do/to 1000) mm	7 μm + 7 · 10 <sup>-4</sup> · L	
	Laserski merilniki razdalje Laser distance meters			- Interni postopek / Internal procedure SOP 34
23.		(0 do/to 50) m	0,8 mm + 24 · 10 <sup>-4</sup> · L	
Končna merila premera / Diameter gauges				
Notranji premer / Internal Diameter				



**SLOVENSKA  
AKREDITACIJA**

Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of  
Akreditacija je veljavna do preklica. Veljavnost preveriti na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at

Priloga k akreditacijski listini  
Annex to Accreditation Certificate

**LK-003**

Velja od / Valid as of

23. marec 2023

10. maj 2022

www.slo-akreditacija.si

Št. No.	Merjena veličina, (pod)področje, oz. merilni instrumenti in/ali območje (merjene veličine). <i>Measured quantity, (sub-)field, and/or instruments, and/or range (of measured quantity).</i>	Območje (merjene veličine) ali Omejitve, pogoji, vplivne veličine.*** <i>Range (of measured quantity) or Limitations, conditions, influence quantity.***</i>	Kalibracijska in merilna zmogljivost (CMC) izražena kot razširjena negotovost.* <i>Calibration and measurement Capability (CMC) Expressed as an Expanded Uncertainty.*</i>	- Tip kalibracijske metode (opcija) - Kalibracijski postopek - Merilni instrumenti (opcija)** - Opombe - Type of calibration method (option), - Internal calibration procedure - Measuring instruments (option)** - Remarks
	Merilni obroči <i>Ring gauges</i>			- Interna postopka / <i>Internal procedures</i> SOP 13, SOP 31
24.		(2 do/to 300) mm	$\sqrt{(0,2 \mu\text{m})^2 + (2,6 \cdot 10^{-6} \cdot L)^2}$	
	<b>Zunanji premer / <i>External Diameter</i></b>			
	Merilni trni in žičke <i>Plugs and wires</i>			- Interna postopka / <i>Internal procedures</i> SOP 14, SOP 31
25.		(0 do/to 50) mm	$0,2 \mu\text{m} + 3 \cdot 10^{-6} \cdot L$	
	Krogle <i>Spheres (balls)</i>			- Interna postopka / <i>Internal procedures</i> SOP 14, SOP 31
26.		(0 do/to 50) mm	$0,2 \mu\text{m} + 3 \cdot 10^{-6} \cdot L$	
	<b>Oblika / <i>Form</i></b>			
	<b>Merila ravnosti / <i>Flatness gauges</i></b>			
	Merilne plošče <i>Surface plates</i>			- Interni postopek / <i>Internal procedure</i> SOP 9
27.		2 m x 3 m	$\sqrt{(0,3 \mu\text{m})^2 + (2 \cdot 10^{-7} \cdot L)^2}$	
	<b>Navojne veličine / <i>Thread quantities</i></b>			
	Navojni trni <i>Thread plugs – plain</i>			- Interni postopek / <i>Internal procedure</i> SOP 10 - Merila / <i>Measures:</i> - valjasti trni / <i>cylindrical gauges</i>
28.	Korak <i>Pitch</i>	(0,25 do/to 7) mm	0,6 $\mu\text{m}$	
29.	Srednji premer <i>Simple pitch diameter</i>	(1 do/to 300) mm	$\alpha = 30^\circ: 4,0 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$ $\alpha = 55^\circ: 3,0 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$ $\alpha = 60^\circ: 3,0 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$ $\alpha = 90^\circ: 2,5 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$	$\alpha =$ bočni kot $\alpha =$ thread angle  Po EURAMET/cg-10, metoda 2a. According to EURAMET/cg-10, method 2a.
	Navojni obroči <i>Thread rings – plain</i>			- Interni postopek / <i>Internal procedure</i> SOP 10 - Merila / <i>Measures:</i> - valjasti obroči / <i>cylindrical gauges</i>
30.	Korak <i>Pitch</i>	(0,25 do/to 6,5) mm	0,8 $\mu\text{m}$	
31.	Srednji premer <i>Simple pitch diameter</i>	(6 do/to 100) mm	$\alpha = 30^\circ: 4,0 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$ $\alpha = 55^\circ: 3,0 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$ $\alpha = 60^\circ: 3,0 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$ $\alpha = 90^\circ: 2,5 \mu\text{m} + 4,5 \cdot 10^{-6} \cdot L$	$\alpha =$ bočni kot $\alpha =$ thread angle  Po EURAMET/cg-10, metoda 2a. According to EURAMET/cg-10, method 2a.
	<b>Koordinatne merilne naprave / <i>Co-ordinate measuring machines</i></b>			
	1D naprave <i>1D measuring machines</i>			- Interni postopek / <i>Internal procedure</i> SOP 7
32.		(0 do/to 5) m	$\sqrt{(30 \text{ nm})^2 + (3,5 \cdot 10^{-4} \cdot L)^2}$	
	Tipalne 3D naprave <i>Tactile 3D machines</i>			- Interni postopek / <i>Internal procedure</i> SOP 18
33.	Odstopanje merjenja dolžine <i>Length measurement deviation</i>	(0 do/to 1) m po osi	$1,0 \mu\text{m} + 2 \cdot 10^{-4} \cdot L$	





**SLOVENSKA  
AKREDITACIJA**

Priloga k akreditacijski listini  
Annex to Accreditation Certificate  
Velja od / Valid as of 23. marec 2023  
Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of 10. maj 2022  
Akreditacija je veljavna do preklica. Veljavnost preveriti na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at  
[www.slo-akreditacija.si](http://www.slo-akreditacija.si)

**LK-003**

23. marec 2023

10. maj 2022

[www.slo-akreditacija.si](http://www.slo-akreditacija.si)

Št. No.	Merjena veličina, (pod)področje, oz. merilni instrumenti in/ali območje (merjene veličine). <i>Measured quantity, (sub-)field, and/or instruments, and/or range (of measured quantity).</i>	Območje (merjene veličine) ali Omejitve, pogoji, vplivne veličine.*** <i>Range (of measured quantity) or Limitations, conditions, influence quantity.***</i>	Kalibracijska in merilna zmogljivost (CMC) izražena kot razširjena negotovost.* <i>Calibration and measurement Capability (CMC) Expressed as an Expanded Uncertainty.*</i>	- Tip kalibracijske metode (opcije) - Kalibracijski postopek - Merilni instrumenti (opcija)** - Opombe - Type of calibration method (option), - Internal calibration procedure - Measuring instruments (option)** - Remarks
34.	Pravokotnost Squareness		1"	
	Optične 3D naprave Optical 3D machines			- Interni postopek / Internal procedure SOP 36
35.		(0 do/to 1) m po osi	3,2 µm + 5,8 · 10 <sup>-6</sup> · L	
	Kot / Angle			
	Merila kota / Angle gauges			
	Kotniki 90° Squares 90°			- Interni postopek / Internal procedure SOP 20
36.		1000 mm x 800 mm	0,9"	
	Merilniki nagiba / Clinometers			
37.		(-3 do/to 3) mm/m (± 600")	1,3 µm/m (0,27")	- Interni postopek / Internal procedure SOP 19
	Lasersko sevanje / Laser radiation			
	Frekvenčno stabilizirani laserji; valovne dolžine v vakuumu Frequency stabilized lasers; vacuum wavelength			- Interni postopek / Internal procedure SOP 32
38.		(632,990 do/to 632,992) nm	10 <sup>9</sup>	Relativna negotovost Relative uncertainty


**SLOVENSKA  
AKREDITACIJA**

Priloga k akreditacijski listini  
Annex to Accreditation Certificate

Velja od / Valid as of  
23. marec 2023

Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of  
10. maj 2022

Akreditacija je veljavna do preklica. Veljavnost preveriti na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at  
www.slo-akreditacija.si

**LK-003**

23. marec 2023

10. maj 2022

[www.slo-akreditacija.si](http://www.slo-akreditacija.si)

Tabela / Table 2 – Kalibracije na terenu / On-site calibrations

Št. No.	Merjena veličina, (pod)področja, oz. merilni instrumenti in/ali območje (merjene veličine). Measured quantity, (sub-)field, and/or instruments, and/or range (of measured quantity).	Območje (merjene veličine) ali Omejitve, pogoji, vplivne veličine.*** Range (of measured quantity) or Limitations, conditions, influence quantity.***	Kalibracijska in merilna zmogljivost (CMC) izražena kot razširjena negotovost.* Calibration and measurement Capability (CMC) Expressed as an Expanded Uncertainty.*	- Tip kalibracijske metode (opcija) - Kalibracijski postopek - Merilni instrumenti (opcija)** - Opombe - Type of calibration method (option), - Internal calibration procedure - Measuring Instruments (option)** - Remarks
<b>DIMENZIONALNE VELIČINE / Dimensional Quantities</b>				
<b>Dolžina / Length (L)</b>				
				L – merjena dolžina / measured length
<b>Instrumenti za merjenje dolžine / Length instruments</b>				
	Naprave za kalibracijo mejnih vzporednih dolžinskih meril Gauge block comparators			- Interni postopek / Internal procedure SOP 2
39.		(0 do/fo 100) mm	$20 \text{ nm} + 0,2 \cdot 10^{-6} \cdot L$	
	Naprave za kalibracijo merilnih uric Dial gauge testers			- Interni postopek / Internal procedure SOP 12
40.		(0 do/fo 125) mm	$0,1 \text{ } \mu\text{m} + 2,5 \cdot 10^{-6} \cdot L$	
<b>Oblika / Form</b>				
	Merilne plošče Surface plates			- Interni postopek / Internal procedure SOP 9
41.		2 m x 3 m	$\sqrt{(0,3 \text{ } \mu\text{m})^2 + (2 \cdot 10^{-7} \cdot L)^2}$	
<b>Koordinatne merilne naprave / Co-ordinate measuring machines</b>				
	1D naprave 1D measuring machines			- Interni postopek / Internal procedure SOP 7
42.		(0 do/fo 5) m	$\sqrt{(30 \text{ nm})^2 + (3,5 \cdot 10^{-6} \cdot L)^2}$	
	Tipalne 3D naprave Tactile 3D machines			- Interni postopek / Internal procedure SOP 18
43.	Odstopanje merjenja dolžine Length measurement deviation	(0 do/fo 1) m po osi	$1,0 \text{ } \mu\text{m} + 2 \cdot 10^{-6} \cdot L$	
44.	Pravokotnost Squareness		1°	
	Optične 3D naprave Optical 3D machines			- Interni postopek / Internal procedure SOP 36
45.		(0 do/fo 1) m po osi	$3,2 \text{ } \mu\text{m} + 5,8 \cdot 10^{-6} \cdot L$	

**Opombe / Notes:**

- \* CMC opomba / CMC Note  
Razširjena negotovost je podana kot kombinirana standardna negotovost pomnožena s takšnim faktorjem pokritja  $k$ , da določa interval zaupanja približno 95 %. / Expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$  such that the coverage probability corresponds to approximately 95 %.
- \*\* Navedba informacije o merilnih instrumentih se v tej koloni uporabi le v tistih primerih, kjer to ne izhaja že iz opredeljene veličine, opisa (pod)področja in instrumentov v drugi koloni tabele. / Information on measuring instruments are specified in this column only if it is not clear from the description of quantity, (sub-) field, and/or instruments in the second column of this table.
- \*\*\* Kadar je za enoumno razumevanje zmogljivosti potreben opis robnih pogojev, vplivnih veličin ali drugih omejitev, se ti navajajo v tej koloni (z enoumno oznako kolona), območje merjene veličine pa je v takem primeru določeno že v drugi koloni te tabele. / When a description of the boundary conditions, influence quantity or other limits is required for an unequivocal understanding of capabilities it is specified in this column (clearly indicated), providing that the range of measured quantity is defined in the second column of this table.



**SLOVENSKA  
AKREDITACIJA**

Priloga k akreditacijski listini  
Annex to Accreditation Certificate

**LK-003**

Velja od / Valid as of

23. marec 2023

Zamenjuje izdajo, veljavno od dne / Replaces the Annex valid as of

10. maj 2022

Akreditacija je veljavna do preklica. Veljavnost preneha na  
This accreditation shall remain in force until withdrawn.  
Information on current status available at

www.slo-akreditacija.si

Datum / Date: 23.3.2023

Direktor / Director

Dr. Boštjan Godec



**SLOVENSKA  
AKREDITACIJA**

Številka norme / Standard number	Opis norme / Description of standard	Področje / Field	Skupna vrednost / Total value
1	Priloga k akreditacijski listini / Annex to accreditation certificate		
2	Priloga k akreditacijski listini / Annex to accreditation certificate		
3	Priloga k akreditacijski listini / Annex to accreditation certificate		
4	Priloga k akreditacijski listini / Annex to accreditation certificate		
5	Priloga k akreditacijski listini / Annex to accreditation certificate		
6	Priloga k akreditacijski listini / Annex to accreditation certificate		
7	Priloga k akreditacijski listini / Annex to accreditation certificate		
8	Priloga k akreditacijski listini / Annex to accreditation certificate		
9	Priloga k akreditacijski listini / Annex to accreditation certificate		
10	Priloga k akreditacijski listini / Annex to accreditation certificate		
11	Priloga k akreditacijski listini / Annex to accreditation certificate		
12	Priloga k akreditacijski listini / Annex to accreditation certificate		
13	Priloga k akreditacijski listini / Annex to accreditation certificate		
14	Priloga k akreditacijski listini / Annex to accreditation certificate		
15	Priloga k akreditacijski listini / Annex to accreditation certificate		
16	Priloga k akreditacijski listini / Annex to accreditation certificate		
17	Priloga k akreditacijski listini / Annex to accreditation certificate		
18	Priloga k akreditacijski listini / Annex to accreditation certificate		
19	Priloga k akreditacijski listini / Annex to accreditation certificate		
20	Priloga k akreditacijski listini / Annex to accreditation certificate		
21	Priloga k akreditacijski listini / Annex to accreditation certificate		
22	Priloga k akreditacijski listini / Annex to accreditation certificate		
23	Priloga k akreditacijski listini / Annex to accreditation certificate		
24	Priloga k akreditacijski listini / Annex to accreditation certificate		
25	Priloga k akreditacijski listini / Annex to accreditation certificate		
26	Priloga k akreditacijski listini / Annex to accreditation certificate		
27	Priloga k akreditacijski listini / Annex to accreditation certificate		
28	Priloga k akreditacijski listini / Annex to accreditation certificate		
29	Priloga k akreditacijski listini / Annex to accreditation certificate		
30	Priloga k akreditacijski listini / Annex to accreditation certificate		
31	Priloga k akreditacijski listini / Annex to accreditation certificate		
32	Priloga k akreditacijski listini / Annex to accreditation certificate		
33	Priloga k akreditacijski listini / Annex to accreditation certificate		
34	Priloga k akreditacijski listini / Annex to accreditation certificate		
35	Priloga k akreditacijski listini / Annex to accreditation certificate		
36	Priloga k akreditacijski listini / Annex to accreditation certificate		
37	Priloga k akreditacijski listini / Annex to accreditation certificate		
38	Priloga k akreditacijski listini / Annex to accreditation certificate		
39	Priloga k akreditacijski listini / Annex to accreditation certificate		
40	Priloga k akreditacijski listini / Annex to accreditation certificate		
41	Priloga k akreditacijski listini / Annex to accreditation certificate		
42	Priloga k akreditacijski listini / Annex to accreditation certificate		
43	Priloga k akreditacijski listini / Annex to accreditation certificate		
44	Priloga k akreditacijski listini / Annex to accreditation certificate		
45	Priloga k akreditacijski listini / Annex to accreditation certificate		
46	Priloga k akreditacijski listini / Annex to accreditation certificate		
47	Priloga k akreditacijski listini / Annex to accreditation certificate		
48	Priloga k akreditacijski listini / Annex to accreditation certificate		
49	Priloga k akreditacijski listini / Annex to accreditation certificate		
50	Priloga k akreditacijski listini / Annex to accreditation certificate		
51	Priloga k akreditacijski listini / Annex to accreditation certificate		
52	Priloga k akreditacijski listini / Annex to accreditation certificate		
53	Priloga k akreditacijski listini / Annex to accreditation certificate		
54	Priloga k akreditacijski listini / Annex to accreditation certificate		
55	Priloga k akreditacijski listini / Annex to accreditation certificate		
56	Priloga k akreditacijski listini / Annex to accreditation certificate		
57	Priloga k akreditacijski listini / Annex to accreditation certificate		
58	Priloga k akreditacijski listini / Annex to accreditation certificate		
59	Priloga k akreditacijski listini / Annex to accreditation certificate		
60	Priloga k akreditacijski listini / Annex to accreditation certificate		
61	Priloga k akreditacijski listini / Annex to accreditation certificate		
62	Priloga k akreditacijski listini / Annex to accreditation certificate		
63	Priloga k akreditacijski listini / Annex to accreditation certificate		
64	Priloga k akreditacijski listini / Annex to accreditation certificate		
65	Priloga k akreditacijski listini / Annex to accreditation certificate		
66	Priloga k akreditacijski listini / Annex to accreditation certificate		
67	Priloga k akreditacijski listini / Annex to accreditation certificate		
68	Priloga k akreditacijski listini / Annex to accreditation certificate		
69	Priloga k akreditacijski listini / Annex to accreditation certificate		
70	Priloga k akreditacijski listini / Annex to accreditation certificate		
71	Priloga k akreditacijski listini / Annex to accreditation certificate		
72	Priloga k akreditacijski listini / Annex to accreditation certificate		
73	Priloga k akreditacijski listini / Annex to accreditation certificate		
74	Priloga k akreditacijski listini / Annex to accreditation certificate		
75	Priloga k akreditacijski listini / Annex to accreditation certificate		
76	Priloga k akreditacijski listini / Annex to accreditation certificate		
77	Priloga k akreditacijski listini / Annex to accreditation certificate		
78	Priloga k akreditacijski listini / Annex to accreditation certificate		
79	Priloga k akreditacijski listini / Annex to accreditation certificate		
80	Priloga k akreditacijski listini / Annex to accreditation certificate		